

**TEST REPORT****IEC 61010-1****Safety requirements for electrical equipment for measurement,
control, and laboratory use****Part 1: General requirements****Report Number.** : LCS210415075AS**Date of issue** : 2021-06-21**Total number of pages** : 66 pages**Name of Testing Laboratory
preparing the Report** : Shenzhen LCS Compliance Testing Laboratory Ltd.
Room 101, 201, Building A and Room 301, Building C, Juji
Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District,
Shenzhen, Guangdong, China**Applicant's name** : Shenzhen Sonoff Technologies Co., Ltd.**Address** : 1001, BLDG8, Lianhua Industrial Park, Shenzhen, GD, China**Test specification:****Standard** : IEC 61010-1:2010, IEC 61010-1:2010/AMD1:2016**Test procedure**..... : Type test**Non-standard test method**..... : N/A**Test Report Form No.**..... : IEC61010_1P**Test Report Form(s) Originator**.... : N/A**Master TRF** : 2021-04-12**Copyright © 2021 IEC System of Conformity Assessment Schemes for Electrotechnical Equipment
and Components (IECEE System). All rights reserved.**

This publication may be reproduced in whole or in part for non-commercial purposes as long as the IECEE is acknowledged as copyright owner and source of the material. IECEE takes no responsibility for and will not assume liability for damages resulting from the reader's interpretation of the reproduced material due to its placement and context.

If this Test Report Form is used by non-IECEE members, the IECEE/IEC logo and the reference to the CB Scheme procedure shall be removed.

**This report is not valid as a CB Test Report unless signed by an approved IECEE Testing Laboratory
and appended to a CB Test Certificate issued by an NCB in accordance with IECEE 02.**

General disclaimer:

The test results presented in this report relate only to the object tested.

This report shall not be reproduced, except in full, without the written approval of the Issuing NCB. The authenticity of this Test Report and its contents can be verified by contacting the NCB, responsible for this Test Report.

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | <http://www.lcs-cert.com>



Test item description: Wi-Fi Smart Switch with Energy Monitoring




Trade Mark: SONOFF

Manufacturer.....: Same as the Applicant

Model/Type reference.....: POWR3

Ratings.....: 100-240V~, 50/60Hz, 25A, Max.load: 5500W

Testing procedure and testing location:

| | | |
|---|----------------------------|---|
| <input checked="" type="checkbox"/> | Testing Laboratory: | Shenzhen LCS Compliance Testing Laboratory Ltd. |
| Testing location/ address | | Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China |
| Tested by (name + signature) | | Tim Liu / Test Engineer  |
| Reviewed by (name + signature) .. | | Caps Li/ Project engineer  |
| Approved by (name + signature) .. | | Hart Qiu/ Technical manager  |

List of Attachments (including a total number of pages in each attachment):

| Document No. | Documents included / attached to this report (description) | Page No. |
|-----------------|--|----------|
| Attachment No.1 | Photos | 6 |

Documents referenced by this report (available on request):

| Document Name or No. | Documents description | Page No. |
|----------------------|-----------------------|----------|
| -- | -- | -- |

Summary of testing:

| Clause | Comment |
|--------|---------|
| N/A | N/A |

Test Report History:

This report may consist of more than one report and is valid only with additional or previous issued reports:

| Ref. No. | Item |
|----------|------|
| N/A | N/A |
| | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | <http://www.lcs-cert.com>

**Tests performed (name of test and test clause):**

The submitted samples were found to comply with the requirements of:

- IEC 61010-1:2010/AMD1:2016
- EN 61010-1:2010+A1:2019

Testing location:


Shenzhen LCS Compliance Testing Laboratory Ltd.
Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Summary of compliance with National Differences

--

Copy of marking plate:

The artwork below may be only a draft. The use of certification marks on a product must be authorized by the respective NCBs that own these marks.

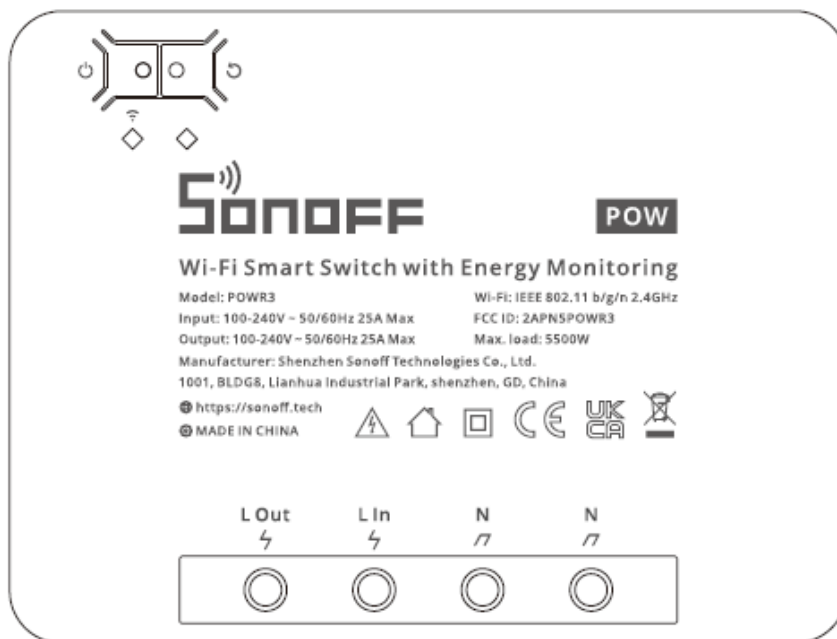**Remarks:**

1. The height dimension of CE mark should not less than 5mm, the height dimension of WEEE symbol should not less than 7mm.



| | |
|--|---|
| Test item particulars: | |
| Type of item | Measurement / Control / Laboratory |
| Description of equipment function..... | |
| Connection to MAINS supply | Permanent / Detachable cord set / Non detachable cord set / None / Battery operated |
| Overvoltage category | II / III / IV |
| POLLUTION DEGREE..... | |
| Means of protection..... | Class I (PE connected) / Class II (isolated) |
| Environmental conditions | Normal / Extended (Specify): |
| For use in wet locations..... | Yes / No |
| Equipment mobility..... | Portable / Hand-held / Floor-standing / Fixed / Built-in |
| Operating conditions..... | Continuous / Short-time / Intermittent |
| Overall size of equipment (W x D x H)..... | |
| Mass of equipment (kg)..... | |
| Marked degree of protection to IEC 60529 | |
| Possible test case verdicts: | |
| - Test case does not apply to the test object | N/A (Not Applicable) |
| - Test object does meet the requirement..... | P (Pass) |
| - Test object does not meet the requirement | F (Fail) |
| Testing: | |
| Date of receipt of test item..... | 2021-04-15 |
| Date (s) of performance of tests | From 2021-04-15 to 2021-05-26 |
| General remarks: | |
| The test results presented in this report relate only to the object tested. This report shall not be reproduced, except in full, without the written approval of the issuing testing laboratory. "(see ENCLOSURE #)" refers to additional information appended to the report. "(see Form A.xx)" refers to a Table appended to the report. Bottom lines for measurement Tables Forms A.xx are optional if used as record. | |
| Throughout this report a <input type="checkbox"/> comma / <input type="checkbox"/> point is used as the decimal separator. | |
| Manufacturer's Declaration per sub-clause 4.2.5 of IEC 60335-1: | |
| The application for obtaining a CB Test Certificate includes more than one factory location and a declaration from the manufacturer stating that the sample(s) submitted for evaluation is (are) representative of the products from each factory has been provided..... | <input type="checkbox"/> Yes <input checked="" type="checkbox"/> Not applicable |
| When differences exist; they shall be identified in the general product information section. | |
| Name and address of factory (ies) | Same as the manufacturer |



General product information and other remarks:

1. The product covered by report is a class II Wi-Fi Smart Switch with Energy Monitoring.



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| | | | |
|-----------|---|---------------------------|-----|
| 4 | TESTS | | |
| 4.4 | Testing in single fault conditions | | P |
| 4.4.1 | Fault tests | (see Form A.1) | P |
| 4.4.2 | Application of single fault conditions | | P |
| 4.4.2.1 | single fault conditions not covered by 4.4.2.2 to 4.4.2.14 | (see Form A.1) | — |
| 4.4.2.2 | Protective impedance | | P |
| 4.4.2.3 | Protective conductor | (see Form A.6) | P |
| 4.4.2.4 | Equipment or parts for short-term or intermittent operation | | N/A |
| 4.4.2.5 | Motors | | — |
| | – stopped while fully energized | | N/A |
| | – prevented from starting | | N/A |
| | – one phase interrupted (multi-phase) | | N/A |
| 4.4.2.6 | Capacitors | | P |
| 4.4.2.7 | Mains transformers | | N/A |
| 4.4.2.7.2 | Short circuit | | P |
| 4.4.2.7.3 | Overload | (see Form A.26B and A.40) | N/A |
| 4.4.2.8 | Outputs | | N/A |
| 4.4.2.9 | Equipment for more than one supply | | N/A |
| 4.4.2.10 | Cooling | (see Form A.26A) | — |
| | – air holes closed | | N/A |
| | – fans stopped | | N/A |
| | – coolant stopped | | N/A |
| | – loss of cooling liquid | | N/A |
| 4.4.2.11 | Heating devices | | N/A |
| | – timer overridden | | N/A |
| | – temperature controller overridden | | N/A |
| 4.4.2.12 | Insulation between circuits and parts | | P |
| 4.4.2.13 | Interlocks | | N/A |
| 4.4.2.14 | Voltage selectors | | N/A |
| 4.4.3 | Duration of tests | (see Form A.1) | — |
| 4.4.4 | Conformity after application of fault conditions | (see Form A.1; A.6, A.18) | P |
| 5 | MARKING AND DOCUMENTATION | | |
| 5.1.1 | Required equipment markings | | — |
| | - Visible from the exterior; or | | P |
| | - Visible after removing cover or opening door | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--|---------------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | - Visible after removal from a rack or panel | | N/A |
| | Not put on parts which can be removed by an operator | | P |
| | Letter symbols (IEC 60027) used | | P |
| | Graphic symbols (IEC 61010-1: Table 1) used | | P |
| 5.1.2 | Identification | | — |
| | Equipment is identified by: | | — |
| | a) Manufacturer's or supplier's name or trademark | See the table | P |
| | b) Model number, name or other means | See the table | P |
| | Manufacturing location identified | Only one manufacturing location | N/A |
| 5.1.3 | Mains supply | | P |
| | Equipment is marked as follows: | | — |
| | a) Nature of supply: | | — |
| | 1) a.c. rated mains frequency or range of frequencies.....: | | — |
| | 2) d.c. with symbol 1 | | P |
| | b) rated supply voltage(s) or range.....: | 100-240V | — |
| | c) Max. rated power (W or VA) or input current | | — |
| | The marked value not less than 90 % of the maximum value | (see Form A.2) | P |
| | If more than one voltage range: | | — |
| | Separate values marked; or | | N/A |
| | Values differ by less than 20 % | (see Form A.2) | P |
| | a) operator-set for different rated supply voltages: | | — |
| | Indicates the equipment set voltage | | N/A |
| | Portable equipment indication is visible from the exterior | | N/A |
| | Changing the setting changes the indication | | N/A |
| | b) Accessory mains socket-outlets accepting standard mains plugs are marked: | | — |
| | With the voltage if it is different from the mains supply voltage.....: | | — |
| | For use only with specific equipment | | N/A |
| | If not marked for specific equipment it is marked with: | | — |
| | The maximum rated current or power; or | | N/A |
| | Symbol 14 with full details in the documentation | | N/A |
| 5.1.4 | Fuses | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Operator replaceable fuse marking (see also 5.4.5).....: | | — |
| 5.1.5 | Terminals, connections and operating devices | | P |
| 5.1.5.1 | General | | — |
| | Where necessary for safety, indication of purpose of terminals, connectors, controls and indicators marked | | P |
| | If insufficient space, symbol 14 used | | P |
| | Push-buttons and actuators of emergency stop devices and indicators: | | — |
| | used only to indicate a warning of danger or | | N/A |
| | the need for urgent action | | N/A |
| | coloured red | | N/A |
| | coded as specified in IEC 60073 | | N/A |
| | Supplementary means of coding provided, if meaning of colour relates (see IEC 60073): | | — |
| | to safety of persons; or | | N/A |
| | safety of the environment | | N/A |
| 5.1.5.2 | terminals | | P |
| | Mains supply terminal identified | | P |
| | Other terminal marking: | | — |
| | a) functional earth terminals (symbol 5 used) | | N/A |
| | b) protective conductor terminals: | | — |
| | Symbol 6 is placed close to or on the terminal; or | | N/A |
| | Part of appliance inlet | | N/A |
| | c) terminals of control circuits (symbol 7 used) | | N/A |
| | d) Hazardous live terminals supplied from the interior | | N/A |
| | Standard mains socket outlet; or | | N/A |
| | Ratings marked; or | | N/A |
| | Symbol 14 used | | N/A |
| 5.1.6 | Switches and circuit breakers | No such devices | N/A |
| | If disconnecting device, off position clearly marked | | N/A |
| | If push-button used as power supply switch: | | — |
| | Symbol 9 and 15 used for on-position | | N/A |
| | Symbol 10 and 16 used for off-position | | N/A |
| | Pair of symbols 9, 15 and 10, 16 close together | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|-------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| 5.1.7 | Equipment protected by double insulation or reinforced insulation | | P |
| | Protected throughout (symbol 11 used) | | P |
| | Only partially protected (symbol 11 not used) | | N/A |
| 5.1.8 | Field-wiring terminal boxes | | N/A |
| | If terminal or enclosure exceeds 60 °C: | (see Form A.26A) | — |
| | Cable temperature rating marked | | — |
| | Marking visible before and during connection or beside terminal | | N/A |
| 5.2 | Warning markings | | P |
| | Visible when ready for normal use | | P |
| | Are near or on applicable parts | | P |
| | Symbols and text correct dimensions and colour: | | — |
| | a) symbols min 2,75 mm and text 1,5 mm high and contrasting in colour with background | | P |
| | b) symbols and text moulded, stamped or engraved in material min. 2,0 mm high and | | P |
| | 0,5 mm depth or raised if not contrasting in colour | | P |
| | If necessary marked with symbol 14 | | P |
| | Statement to isolate or disconnect if access by using a tool to hazardous live parts is permitted | | N/A |
| 5.3 | Durability of markings | | P |
| | The required markings remain clear and legible in normal use | (see Form A.3) | P |
| 5.4 | Documentation | English manual provided | P |
| 5.4.1 | General | | P |
| | Equipment is accompanied by documentation for safety purposes for operator or responsible body | | P |
| | Safety documentation for service personnel authorized by the manufacturer | | P |
| | Documentation necessary for safe operation is provided in printed media or | | P |
| | in electronic media if available at any time | | N/A |
| | Documentation includes: | | — |
| | a) intended use | | P |
| | b) technical specification | | P |
| | c) name and address of manufacturer or supplier | | P |
| | d) information specified in 5.4.2 to 5.4.6 | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | e) information to mitigate residual risk (see also subclause 17) | | N/A |
| | f) accessories for safe operation of the equipment specified | | N/A |
| | g) guidance provided to check correct function of the equipment, if incorrect reading may cause a hazard from harmful or corrosive substances of hazardous live parts | | P |
| | h) instructions for lifting and carrying | <18kg | N/A |
| | Warning statements and a clear explanation of warning symbols: | | P |
| | Provided in the documentation; or | | P |
| | Information is marked on the equipment | | N/A |
| 5.4.2 | Equipment ratings | | P |
| | Documentation includes: | | — |
| | a) Supply voltage or voltage range | 100-240V~ | — |
| | Frequency or frequency range | | — |
| | Power or current rating | 25A | — |
| | b) Description of all input and output connections in accordance to 6.6.1 a) | | P |
| | c) rating of insulation of external circuits in accordance to 6.6.1 b) | | N/A |
| | d) Statement of the range of environmental conditions (see 1.4) | | P |
| | e) Degree of protection (IEC 60529) | IPX0 | N/A |
| | f) If impact rating less than 5 J: | | — |
| | IK code in accordance to IEC 62262 marked or | | N/A |
| | symbol 14 of table 1 marked, with | | N/A |
| | rated energy level and test method stated | | N/A |
| 5.4.3 | Equipment installation | | P |
| | Documentation includes instructions for: | | — |
| | a) assembly, location and mounting requirements | | P |
| | b) protective earthing | | N/A |
| | c) connections to supply | | P |
| | d) permanently connected equipment: | | — |
| | 1) Supply wiring requirements | | N/A |
| | 2) If external switch or circuit-breaker, requirements and location recommendation | | N/A |
| | e) ventilation requirements | | N/A |
| | f) special services (e. g. air, cooling liquid) | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|--------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | g) instructions relating to sound level | | N/A |
| 5.4.4 | Equipment operation | | P |
| | Instructions for use include: | | — |
| | a) identification and description of operating controls | | P |
| | b) positioning for disconnection | | N/A |
| | c) instructions for interconnection | | P |
| | d) specification of intermittent operation limits | | N/A |
| | e) explanation of symbols used | | P |
| | f) replacement of consumable materials | Details see instructions | P |
| | g) cleaning and decontamination | | P |
| | h) listing of any poisonous or injurious gases and quantities | | N/A |
| | i) risk reduction procedures relating to flammable liquids (see 9.5) | | N/A |
| | j) risk reduction procedures relating burn from surfaces permitted to exceed limits of 10.1 | | N/A |
| | Additional precautions for IEC 60950 conforming equipment in regard to moistures and liquids | | N/A |
| | A statement about protection impairment if used in a manner not specified by the manufacturer | | P |
| 5.4.5 | Equipment maintenance and Service | | P |
| | Instructions for responsible body include: | | — |
| | Instructions sufficient in detail permitting safe maintenance and inspection and continued safety: | | — |
| | Instruction against the use of detachable mains supply cord with inadequate rating | | P |
| | Specific battery type of user replaceable batteries | | P |
| | Any manufacturer specified parts | | P |
| | Rating and characteristics of fuses | | P |
| | Instructions include following subjects permitting safe servicing and continued safety: | | — |
| | a) product specific risks may affect service personnel | | P |
| | b) protective measures for these risks | | P |
| | c) verification of the safe state after repair | | P |
| 5.4.6 | Integration into systems or effects resulting from special conditions | | N/A |
| | Aspects described in documentation | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--|--------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| 6 | PROTECTION AGAINST ELECTRIC SHOCK | | |
| 6.1 | General | (see Form A.14 and A.15) | P |
| 6.1.1 | Requirements | | — |
| | Protection against electric shock maintained in normal condition and single fault condition | | P |
| | accessible parts not hazardous live | | P |
| | Voltage, current, charge or energy below the limits in normal condition and in single fault condition between: | | — |
| | accessible parts and earth | | P |
| | two accessible parts on same piece of the equipment within a distance of 1,8 m | | P |
| | Conformity is checked by the determination of 6.2 and 6.3 followed by the tests of 6.4 to 6.11 | | P |
| 6.1.2 | Exceptions | | N/A |
| | Following hazardous live parts may be accessible to an operator: | | — |
| | a) parts of lamps and lamp sockets after lamp removal | | N/A |
| | b) parts to be replaced by operator only by the use of tool and warning marking | Marked with symbol | P |
| | Those parts not hazardous live 10 s after interruption of supply | | N/A |
| | Capacitance test if charge is received from internal capacitor | | N/A |
| 6.2 | Determination of accessible parts | | P |
| 6.2.1 | General | | P |
| | Unless obviously determination of accessible parts as specified in 6.2.2 to 6.2.4 | | P |
| 6.2.2 | Examination | | N/A |
| | - with jointed test finger (as specified B.2) | | N/A |
| | - with rigid test finger (as specified B.1) and a force of 10 N | | N/A |
| 6.2.3 | Openings above parts that are hazardous live | | N/A |
| | - test pin with length of 100 mm and 4 mm in diameter applied | | N/A |
| 6.2.4 | Openings for pre-set controls | | N/A |
| | - test pin with length of 100 mm and 3 mm in diameter applied | | N/A |
| 6.3 | Limit values for accessible parts | | P |
| 6.3.1 | Levels in normal condition | (see Form A.5) | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|--------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | a) Voltage limits less than 33 V r.m.s. and 46,7 V peak or 70 V d.c. | | P |
| | for wet locations voltage limits less than 16 V r.m.s. and 22,6 V peak or 35 V d.c. | | N/A |
| | Voltages are not hazardous live the levels of: | | — |
| | b) Current less than 0,5 mA r.m.s. for sinusoidal, 0,7 mA peak non sinusoidal or mixed frequencies or 2 mA d.c. when measured with measuring circuit A.1 or A.2 if less than 100 Hz | A.1 | P |
| | for wet locations measuring circuit A.4 used | | N/A |
| | 70 mA r.m.s. when measured with circuit A.3 for higher frequencies | | N/A |
| | or | | — |
| | c) Levels of capacitive charge or energy less: | | — |
| | 1) 45 μ C for voltages up to 15 kV peak or d.c. or line A of Figure 3 | | P |
| | 2) 350 mJ stored energy for voltages above 15 kV peak or d.c. | | N/A |
| 6.3.2 | Levels in single fault condition | (see Form A.6) | — |
| | a) Voltage limits less than 55 V r.m.s. and 78 V peak or 140 V d.c. | | P |
| | for wet locations voltage limits less than 33 V r.m.s. and 46,7 V peak or 70 V d.c. | | N/A |
| | Voltages are not hazardous live the levels of: | | — |
| | b) Current less than 3,5 mA r.m.s. for sinusoidal, 5 mA peak non sinusoidal or mixed frequencies or 15 mA d.c. when measured with measuring circuit A.1 or A.2 if less than 100 Hz | A.1 | P |
| | for wet locations measuring circuit A.4 used | | N/A |
| | 500 mA r.m.s. when measured with circuit A.3 for higher frequencies | | N/A |
| | or | | — |
| | c) Levels of capacitive charge or energy less line B of Figure 3 | | P |
| 6.4 | Primary means of protection | | P |
| 6.4.1 | Accessible parts prevented from being hazardous live by one or more of following means: | | — |
| | a) enclosures or protective barriers (see 6.4.2) | | P |
| | b) basic insulation (see 6.4.3) | | N/A |
| | c) Impedance (see 6.4.4) | | P |
| 6.4.2 | enclosures or protective barriers | (see Form A.15 and A.16) | — |
| | - meet rigidity requirements of 8.1 | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|--|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | - meet requirements for basic insulation, if protection is provided by insulation | | N/A |
| | - meet requirements of 6.7 for creepage and clearances between accessible parts and hazardous live parts, if protection is provided by limited access | | P |
| 6.4.3 | Basic insulation | (see Form A.15 and A.16) | — |
| | - meet clearance, creepage distance and solid insulation requirements of 6.7 | | N/A |
| 6.4.4 | Impedance | (see Form A.12 and A.16) | — |
| | Impedance used as primary means of protection meets all of following requirements: | | — |
| | a) limits current or voltage to level of 6.3.2 | (see Form A.6) | P |
| | b) rated for maximum working voltage and the amount of power it will dissipate | | P |
| | c) clearance, creepage distance between terminations of the impedance meet requirements of basic insulation of 6.7 | (see Form A.15) | P |
| 6.5 | Additional means of protection in case of single fault condition | | P |
| 6.5.1 | Accessible parts are prevented from becoming hazardous live by the primary means of protection and supplemented by one of: | | — |
| | a) protective bonding (see 6.5.2) | | N/A |
| | b) supplementary insulation (see 6.5.3) | | N/A |
| | c) automatic disconnection of the supply (see 6.5.5) | | N/A |
| | d) current- or voltage-limiting device (see 6.5.6) | | N/A |
| | Alternatively one of the single means of protection is used: | | — |
| | e) reinforced insulation (see 6.5.3) | | P |
| | f) protective impedance (see 6.5.4) | | P |
| 6.5.2 | Protective bonding | (see Form A.7, A.8, A.9, A.10 or A.11) | P |
| 6.5.2.1 | Accessible conductive parts, may become hazardous live in single fault condition: | | — |
| | Bonded to the protective conductor terminal; or | | N/A |
| | Separated by conductive screen or barrier bonded to protective conductor terminal | | N/A |
| 6.5.2.2 | Integrity of protective bonding | | — |
| | a) protective bonding consists of directly connected structural parts or discrete conductors or both; and withstands thermal and dynamic stresses | | P |
| | b) Soldered connections: | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Independently secured against loosening | | N/A |
| | Not used for other purposes | | N/A |
| | c) Screw connections are secured | | N/A |
| | d) protective bonding not interrupted; or | | P |
| | exempted as removable part carries mains supply input connection | | N/A |
| | e) Any movable protective bonding connection specifically designed, and meets 6.5.2.4 | | N/A |
| | f) No external metal braid of cables used (not regarded as protective bonding) | | N/A |
| | g) If mains supply passes through: | | — |
| | Means provided for passing protective conductor; | | N/A |
| | Impedance meets 6.5.2.4 | | N/A |
| | h) Protective conductors bare or insulated, if insulated, green/yellow | | P |
| | Exceptions: | | — |
| | 1) earthing braids; | | N/A |
| | 2) internal protective conductors etc.; | | N/A |
| | Green/yellow not used for other purposes | | N/A |
| | terminal suitable for connection of a protective conductor, and meets 6.5.2.3 | | N/A |
| 6.5.2.3 | Protective conductor terminal | | — |
| | a) Contact surfaces are metal | | P |
| | b) Appliance inlet used | | N/A |
| | c) For rewirable cords and permanently connected equipment, protective conductor terminal is close to mains supply terminals | | P |
| | d) If no mains supply is required, any protective conductor terminal: | | — |
| | Is near terminals of circuit for which protective earthing is necessary | | N/A |
| | External if other terminals external | | N/A |
| | e) Equivalent current-carrying capacity to mains supply terminals | | N/A |
| | f) If plug-in, makes first and breaks last | | N/A |
| | g) If also used for other bonding purposes, protective conductor: | | — |
| | Applied first; | | N/A |
| | Secured independently; | | N/A |
| | Unlikely to be removed by servicing | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|-----------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | h) Protective conductor of measuring circuit: | | — |
| | 1) Current rating equivalent to measuring circuit terminal; | | P |
| | 2) protective bonding: not interrupted by any switch or interrupting device | | N/A |
| | i) functional earth terminals allow independent connection | | N/A |
| | j) If a binding screw used for Protective conductor terminal: | | — |
| | Suitable size for bond wire | | P |
| | Not smaller than M 4 | | P |
| | At least 3 turns of screw engaged | | P |
| | Passes tightening torque test | (see Form A.8) | P |
| | k) Contact pressure not capable being reduced by deformation of materials | | P |
| 6.5.2.4 | Impedance of protective bonding of plug-connected equipment | (see Form A.9) | — |
| | Impedance between protective conductor terminal and each accessible part where protective bonding is specified, is: | | — |
| | less than 0,1 Ohm; or | | P |
| | less than 0,2 Ohm if equipment is provided with non detachable cord | | N/A |
| 6.5.2.5 | Bonding impedance of permanently connected equipment | (see Form A.10) | — |
| 6.5.2.6 | Transformer protective bonding screen | (see Form A.11) | — |
| | Transformer provided with screen for protective bonding: | | — |
| | screen bonding consists of directly connected structural parts or discrete conductors or both; and withstands thermal and dynamic stresses (see 6.5.2.2 a) | | N/A |
| | screen bonding with soldered connection (see 6.5.2.2 b) is: | | N/A |
| | - Independently secured against loosening | | N/A |
| | - Not used for other purposes | | N/A |
| 6.5.3 | Supplementary and reinforced insulation | Reinforced insulation | P |
| | Meet clearance, creepage distance and solid insulation requirements of 6.7 | | P |
| 6.5.4 | Protective impedance | (see Form A.12) | P |
| | Limits current or voltage to level of 6.3.1 in normal and to level of 6.3.2 in single fault condition | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--|-----------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | clearance, creepage distance between terminations of the impedance meet requirements of double or reinforced insulation of 6.7 | (see Form A.15) | P |
| | The protective impedance consists of one or more of the following: | (see TABLE 1 and Form A.12) | — |
| | a) appropriate single component suitable for safety and reliability for protection, it is: | | — |
| | 1) rated twice the maximum working voltage | | N/A |
| | 2) resistor rated for twice the power dissipation for maximum working voltage | | N/A |
| | b) combination of components | | P |
| | Single electronic device not used as protective impedance | | P |
| 6.5.5 | Automatic disconnection of the supply | | N/A |
| | a) rated to disconnect the load within time specified in Figure 2 | | N/A |
| | b) rated for the maximum load conditions of the equipment | | N/A |
| 6.5.6 | Current- or voltage-limiting devices | | N/A |
| | Device complies with all of: | | — |
| | a) rated to limit the current or voltage to the level of 6.3.2 | | N/A |
| | b) rated for the maximum working voltage; and | | N/A |
| | rated for the maximum operational current if applicable | | N/A |
| | c) clearance, creepage distance between terminations of the impedance meet requirements of supplementary insulation of 6.7 | | N/A |
| 6.6 | Connections to external circuits | | P |
| 6.6.1 | Connections do not cause accessible parts of the following to become hazardous live in normal condition or single fault condition: | | — |
| | - the external circuits | | P |
| | - the equipment | | P |
| | Protection achieved by separation of circuits; or | | P |
| | short circuit of separation does not cause a hazard | | N/A |
| | Instructions or markings for each terminal include: | | — |
| | a) rated conditions for terminal | | P |
| | b) Required rating of external circuit insulation | | N/A |
| 6.6.2 | Terminals for external circuits | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Terminals which receive a charge from an internal capacitor are not hazardous live after 10 s of interrupting supply connection | (see Form A.5) | N/A |
| 6.6.3 | Circuits with terminals which are hazardous live | | P |
| | These circuits are: | | — |
| | Not connected to accessible conductive parts; or | | P |
| | Connected to accessible conductive parts, but are not mains circuits and have one terminal contact at earth potential | | N/A |
| | No accessible conductive parts are hazardous live | | P |
| 6.6.4 | Accessible terminals for stranded conductors | | N/A |
| | No risk of accidental contact because: | | — |
| | Located or shielded | | N/A |
| | Self-evident or marked whether or not connected to accessible conductive parts | | N/A |
| | Accessible terminals will not work loose | | N/A |
| 6.7 | Insulation requirements | (see Form A.14) | P |
| 6.7.1 | The nature of insulation | | — |
| 6.7.1.1 | Insulation between accessible parts or between separate circuits consist of clearances, creepage distances and solid insulation if provided as protection against a hazard | | P |
| 6.7.1.2 | Clearances | | — |
| | Required clearances reflecting factors of 6.7.1.1 | (see Form A.14, A.15) | P |
| | Equipment rated for operating altitude greater than 2000 m correction factor of Table 3 of 61010-1 applied | ≤3000m | P |
| 6.7.1.3 | Creepage distances | | — |
| | Required creepage distances reflecting factors of 6.7.1.1 a) to d) | (see Form A.14, A.15) | P |
| | CTI material group reflected by requirements | | P |
| | CTI test performed | | N/A |
| 6.7.1.4 | Solid insulation | | — |
| | Required solid insulation reflecting factors of 6.7.1.1 a) to d) | (see Form A.14, A.15) | P |
| 6.7.1.5 | Requirements for insulation according to type of circuit | (see Form A.14, A.15) | — |
| | a) 6.7.2 mains circuits of overvoltage category II up to nominal supply voltage of 300 V | | N/A |
| | b) 6.7.3 secondary circuits separated from circuits defined in a) by transformer | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|-----------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | c) K.1 mains circuits of overvoltage category III and IV or overvoltage category II over 300 V | | N/A |
| | d) K.2 secondary circuits separated from circuits defined in c) by transformer | | N/A |
| | e) K.3 circuits having one or more of: | | — |
| | 1) maximum transient overvoltage is limited to known level below the level of mains circuit | | P |
| | 2) maximum transient overvoltage above the level of mains circuit | | N/A |
| | 3) Working voltage is the sum of more than one circuit or a mixed voltage | | N/A |
| | 4) Working voltage includes recurring peak voltage, may include non-sinusoidal or non-periodic waveform | | N/A |
| | 5) Working voltage with a frequency above 30 kHz | | N/A |
| 6.7.2 | Insulation for mains circuits of overvoltage category II with a nominal supply voltage up to 300 V | | P |
| 6.7.2.1 | Clearances and creepage distances | (see Form A.14, A.15) | — |
| | Values for mains circuits of Table 4 are met | | P |
| | Coatings to achieve reduction to pollution degree 1 comply with requirements of Annex H | | N/A |
| 6.7.2.2 | Solid insulation | | P |
| 6.7.2.2.1 | Withstands electrical and mechanical stresses in normal use and all rated environmental conditions of 1.4 | | — |
| | Equipment passed voltage tests of 6.8.3 with values of Table 5 | (see Form A.18) | N/A |
| | Complies as applicable: | | — |
| | a) enclosure or protective barrier of Clause 8 | | P |
| | b) moulded and potted parts requirements of 6.7.2.2.2 | | N/A |
| | c) inner layers of printed wiring boards requirements of 6.7.2.2.3 | | P |
| | d) thin-film insulation requirements of 6.7.2.2.4 | | P |
| 6.7.2.2.2 | Moulded and potted parts | | — |
| | Conductors between same two layers are separated by at least 0,4 mm after moulding is completed | | N/A |
| 6.7.2.2.3 | Inner insulating layers of printed wiring boards | | — |
| | Separated by at least 0,4 mm between same two layers | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Reinforced insulation have adequate electric strength; one of following methods used: | | — |
| | a) thickness of insulation is at least 0,4 mm | | P |
| | b) insulation is assembled of minimum two separate layers, each rated for test voltage of Table 5 for basic insulation | | N/A |
| | c) insulation is assembled of minimum two separate layers, where the combination is rated for test voltage of Table 5 for reinforced insulation | | P |
| 6.7.2.2.4 | Thin-film insulation | | — |
| | Conductors between same two layers are separated by applicable clearances and creepage distance of 6.7.2.1 | | P |
| | Reinforced insulation have adequate electric strength; one of following methods used: | | — |
| | a) thickness through the insulation at least 0,4 mm | | P |
| | b) insulation is assembled of min two separate layers, each rated for test voltage of Table 5 for basic insulation | | N/A |
| | c) insulation is assembled of min three separate layers, where the combination of two layers passed voltage tests of 6.8.3 with values of Table 5 for reinforced insulation | (see Form A.18) | P |
| 6.7.3 | Insulation for secondary circuits derived from mains circuits of overvoltage category II up to 300 V | No such circuits | N/A |
| 6.7.3.1 | Secondary circuits where separation from mains circuits is achieved by a transformer providing: | | — |
| | - reinforced insulation | | P |
| | - double insulation | | N/A |
| | - screen connected to the protective conductor terminal | | N/A |
| 6.7.3.2 | Clearances | | — |
| | a) meet the values of Table 6 for basic insulation and supplementary insulation; or | | P |
| | twice the values of Table 6 for reinforced insulation | | P |
| | or | | — |
| | b) pass the voltage tests of 6.8 with values of Table 6; | (see Form A.18) | — |
| | with following adjustments: | | — |
| | 1) values for reinforced insulation are 1,6 times the values for basic insulation | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | 2) if operating altitude is greater than 2000 m values of clearances multiplied with factor of Table 3 | | P |
| | 3) minimum clearance is 0,2 mm for pollution degree 2 and 0,8 mm for pollution degree 3 | | P |
| 6.7.3.3 | Creepage distances | | — |
| | Based on working voltage meets the values of Table 7 for basic and supplementary insulation | | P |
| | Values for reinforced insulation are twice the values of basic insulation | | P |
| | Coatings to achieve reduction to pollution degree 1 comply with requirements of Annex H | | N/A |
| 6.7.3.4 | Solid insulation | | — |
| 6.7.3.4.1 | Withstands electrical and mechanical stresses in normal use and all rated environmental conditions of 1.4 | | — |
| | a) Equipment passed voltage test of 6.8.3.1 for 5 s with values of Table 6 for basic and supplementary insulation | (see Form A.18) | P |
| | values for reinforced insulation are 1,6 times the values of basic insulation | | P |
| | b) if working voltage exceeds 300 V, equipment passed voltage test of 6.8.3.1 for 1 min with a test voltage of 1,5 times working voltage for basic or supplementary insulation | (see Form A.18) | N/A |
| | value for reinforced insulation are twice the working voltage | | N/A |
| | Complies as applicable: | | — |
| | 1) enclosure or protective barrier of Clause 8 | | N/A |
| | 2) moulded and potted parts requirements of 6.7.3.4.2 | | N/A |
| | 3) inner layers of printed wiring boards requirements of 6.7.3.4.3 | | N/A |
| | 4) thin-film insulation requirements of 6.7.3.4.4 | | N/A |
| 6.7.3.4.2 | Moulded and potted parts | | — |
| | Conductors between same two layers are separated by applicable distances of Table 8 | | N/A |
| 6.7.3.4.3 | Inner insulation layers of printed wiring boards | | — |
| | Separated by at least by applicable distances of Table 8 between same two layers | | N/A |
| | Reinforced insulation have adequate electric strength; one of following methods used: | | — |
| | a) thickness at least applicable distance of Table 8 | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|--------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | b) insulation is assembled of minimum two separate layers, each rated for test voltage of Table 6 for basic insulation | | N/A |
| | c) insulation is assembled of min two separate layers, where the combination is rated for 1,6 times the test voltage of Table 6 | | N/A |
| 6.7.3.4.4 | Thin-film insulation | | — |
| | Conductors between same two layers are separated by applicable clearances and creepage distance of 6.7.3.2 and 6.7.3.3 | | N/A |
| | Reinforced insulation have adequate electric strength; one of following methods used: | | — |
| | a) thickness at least applicable distance of Table 8 | | N/A |
| | b) insulation is assembled of min two separate layers, each rated for test voltage of Table 6 for basic insulation | | N/A |
| | c) insulation is assembled of min three separate layers, where the combination of two layers passed voltage tests with 1,6 time values of Table 6: | (see Form A.18) | — |
| | a.c. test of 6.8.3.1; or | | N/A |
| | d.c. test of 6.8.3.2 for circuits stressed only by d.c. voltages | | N/A |
| 6.8 | Procedure for dielectric strength tests | (see Form A.14 and A.18) | P |
| 6.9 | Constructional requirements for protection against electric shock | | P |
| 6.9.1 | If a failure could cause a hazard: | | — |
| | a) Security of wiring connections | | P |
| | b) Screws securing removable covers | | P |
| | c) Accidental loosening | | P |
| | d) clearances and creepage distances not reduced below the values of basic insulation by loosening of parts or wires | | P |
| 6.9.2 | Insulating materials | | P |
| | Material not to be used for safety relevant insulation: | | — |
| | a) Easily damaged materials not used | | P |
| | b) Non-impregnated hygroscopic materials not used | | P |
| 6.9.3 | Colour coding | | P |
| | Green-and-yellow insulation shall not be used except: | | — |
| | a) protective earth conductors; | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | b) protective bonding conductors; | | P |
| | c) potential equalization conductors; | | N/A |
| | d) functional earth conductors | | N/A |
| 6.10 | Connection to mains supply source and connections between parts of equipment | | P |
| 6.10.1 | Mains supply cords | | — |
| | rated for maximum equipment current (see 5.1.3 c) | | P |
| | Cable complies with IEC 60227 or IEC 60245 | | P |
| | Heat-resistant if likely to contact hot parts | | N/A |
| | Temperature rating (cord and inlet) | | — |
| | Green/yellow used only for connection to protective conductor terminals | | P |
| | Detachable cords with IEC 60320 mains connectors: | | — |
| | Conform to IEC 60799; or | | P |
| | Have the current rating of the mains connector | | N/A |
| 6.10.2 | Fitting of non-detachable mains supply cords | | — |
| 6.10.2.1 | Cord entry | | — |
| | a) Inlet or bushing with a smoothly rounded opening; or | | N/A |
| | b) Insulated cord guard protruding >5 D | | N/A |
| 6.10.2.2 | Cord anchorage | | — |
| | Protective earth conductor is the last to take the strain | | N/A |
| | a) Cord is not clamped by direct pressure from a screw | | N/A |
| | b) Knots are not used | | N/A |
| | c) Cannot push the cord into the equipment to cause a hazard | | N/A |
| | d) No failure of cord insulation in anchorage with metal parts | | N/A |
| | e) Not to be loosened without a tool | | N/A |
| | f) Cord replacement does not cause a hazard and method of strain relief is clear | | N/A |
| | Push-pull and or torque test | (see Form A.19) | N/A |
| 6.10.3 | Plugs and connectors | | P |
| | Mains supply plugs, connectors etc., conform with relevant specifications | | P |
| | If equipment supplied at voltages below 6.3.2.a) or from a sole source: | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Plugs of supply cords do not fit mains sockets above rated supply voltage | | N/A |
| | Mains type plugs used only for connection to mains supply | | N/A |
| | Plug pins which receive a charge from an internal capacitor | (see Form A.5) | N/A |
| | Accessory mains socket outlets: | | — |
| | a) Marking if accepts a standard mains supply plug (see 5.1.3e) | | N/A |
| | b) Input has a protective earth conductor if outlet has earth terminal contact | | N/A |
| 6.11 | Disconnection from supply source | AC inlet | P |
| 6.11.1 | Disconnects all current-carrying conductors | | P |
| 6.11.2 | Exceptions | | N/A |
| 6.11.3 | Requirements according to type of equipment | | — |
| 6.11.3.1 | Permanently connected equipment and multi-phase equipment | | N/A |
| | Employs switch or circuit-breaker | | N/A |
| | If switch or circuit-breaker is not part of the equipment, documentation requires: | | — |
| | a) Switch or circuit-breaker to be included in building installation | | N/A |
| | b) Suitable location easily reached | | N/A |
| | c) Marking as disconnecting for the equipment | | N/A |
| 6.11.3.2 | Single-phase cord-connected equipment | | — |
| | Equipment is provided with one of the following: | | P |
| | a) Switch or circuit-breaker | | P |
| | b) Appliance coupler (disconnectable without tool) | | N/A |
| | c) Separable plug (without locking device) | | N/A |
| 6.11.4 | Disconnecting devices | | P |
| 6.11.4.1 | Disconnecting device part of equipment | | P |
| | Electrically close to the supply | | N/A |
| | Power-consuming components not electrically located between the supply source and the disconnecting device | | N/A |
| | Except electromagnetic interference suppression circuits permitted to be located on the supply side of the disconnecting device | | N/A |
| 6.11.4.2 | Switches and circuit-breakers | | P |
| | When used as disconnection device: | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| | | | |
|----------|--|--|-----|
| | Meets IEC 60947-1 and IEC 60947-3 | | P |
| | Marked to indicate function.....: | | — |
| | Not incorporated in mains cord | | N/A |
| | Does not interrupt protective earth conductor | | N/A |
| 6.11.4.3 | Appliance couplers and plugs | | P |
| | Where an appliance coupler or separable plug is used as the disconnecting device (see 6.11.3.2): | | — |
| | Readily identifiable and easily reached by the operator | | P |
| | Single-phase portable equipment cord length not more than 3 m | | N/A |
| | Protective earth conductor connected first and disconnected last | | P |

| | | | |
|-------|---|----------------|-----|
| 7 | PROTECTION AGAINST MECHANICAL HAZARDS | | |
| 7.1 | Equipment does not cause a mechanical hazard in normal nor in single fault condition | | P |
| | Conformity is checked by 7.2 to 7.7 | | P |
| 7.2 | Sharp edges | | P |
| | Easily touched parts are smooth and rounded | | P |
| | Do not cause injury during normal use and | | P |
| | Do not cause injury during single fault condition | | P |
| 7.3 | Moving parts | No moving part | N/A |
| 7.3.1 | Hazards from moving parts limited to a tolerable level with the conditions specified in 7.3.2 and 7.3.5 | | N/A |
| | Risk assessment in accordance with 7.3.3 carried out | | N/A |
| 7.3.2 | Exceptions | | N/A |
| | Access to hazardous moving parts permitted under following circumstances: | | — |
| | a) obviously intended to operate on parts or materials external of the equipment | | N/A |
| | inadvertent touching of moving parts minimized by equipment design (e.g. guards or handles) | | N/A |
| | b) If operator access is unavoidable outside normal use following precautions have been taken: | | — |
| | 1) Access requires tool | | N/A |
| | 2) Statement about training in the instructions | | N/A |
| | 3) Warning markings on covers prohibiting access by untrained operators | | N/A |
| | or symbol 14 with full details in documentation | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| 7.3.3 | Risk assessment for mechanical hazards to body parts | | N/A |
| | Risk is reduced to a tolerable level by protective measures as specified in table 12 | | N/A |
| | Minimum protective measures: | | — |
| | A. Low level measures | | N/A |
| | B. Moderate measures | | N/A |
| | C. Stringent measures | | N/A |
| 7.3.4 | Limitation of force and pressure | (see Form A.20) | N/A |
| | Following levels are met in normal and single fault condition: | | — |
| | Continuous contact pressure below 50 N / cm ² with force below 150 N | | N/A |
| | Temporary force below 250 N for an area at least of 3 cm ² for a maximum duration of 0,75 s | | N/A |
| 7.3.5 | Gap limitations between moving parts | | N/A |
| 7.3.5.1 | Access normally allowed | | — |
| | If levels of 7.3.4 exceeded and body part may be inserted minimum gap as specified in table 13 assured in normal and in single fault condition | | N/A |
| 7.3.5.2 | Access normally prevented | | — |
| | Maximum gap as specified in table 14 assured in normal and in single fault condition | | N/A |
| 7.4 | Stability | | P |
| | Equipment not secured to building structure is physical stable | | P |
| | Stability maintained after opening of drawers etc. by automatic means, or | | N/A |
| | warning marking requires the application of means | | N/A |
| | Compliance checked by following tests as applicable: | | — |
| | a) 10° tilt test for other than handheld equipment | | P |
| | b) multi-directional force test for equipment exceeds height of 1 m and mass of 25 kg | | N/A |
| | c) downward force test for floor-standing equipment | | N/A |
| | d) overload test with 4 times maximum load for castor or support that supports greatest load | | N/A |
| | e) castor or support that supports greatest load removed from equipment | | N/A |
| 7.5 | Provisions for lifting and carrying | <18kg | N/A |
| 7.5.1 | Equipment more than 18 kg : | | — |
| | Has means for lifting or carrying; or | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| | | | |
|-------|--|--|-----|
| | Directions in documentation | | N/A |
| 7.5.2 | Handles and grips | | — |
| | Handles or grips withstand four times weight | | N/A |
| 7.5.3 | Lifting devices and supporting parts | | — |
| | Rated for maximum load; or | | N/A |
| | tested with four times maximum static load | | N/A |
| 7.6 | Wall mounting | | P |
| | Mounting brackets withstand four times weight | | P |
| 7.7 | Expelled parts | | P |
| | Equipment contains or limits the energy | | P |
| | Protection not removable without the aid of a tool | | P |

| | | | |
|-----|---|--|-----|
| 8 | RESISTANCE TO MECHANICAL STRESSES | | |
| 8.1 | Equipment does not cause a hazard when subjected to mechanical stresses in normal use | | P |
| | Normal protection level is 5 J | | P |
| | Levels below 5 J but not less than 1 J are acceptable if all of following criteria are met: | | — |
| | a) lower level justified by risk assessment of manufacturer | | N/A |
| | b) equipment installed in its intended application is not easily touched | | N/A |
| | c) only occasional access during normal use | | N/A |
| | d) IK code in accordance to IEC 62262 marked or symbol 14 used with full information in the documentation | | N/A |
| | For non-metallic enclosures rated below 2 °C ambient temperature value chosen for minimum rated temperature | | N/A |
| | Impact energies between IK values, the IK code marked for nearest lower value | | N/A |
| | Conformity is checked by performing following tests: | | — |
| | 1) static test of 8.2.1 | | P |
| | 2) impact test of 8.2.2 with 5 J except for hand-held equipment | | P |
| | if impact energy not selected to 5 J alternate method of IEC 62262 used | | N/A |
| | 3) drop test of 8.3.1 or 8.3.2 except for fixed equipment and equipment with mass over 100 kg | | N/A |
| | Equipment rated with an impact rating of IK 08 that obviously meets the criteria | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| | | | |
|-------|---|------------------|-----|
| | After the tests inspection with following results: | | — |
| | - hazardous live parts above the limits of 6.3.2 not accessible | | P |
| | - insulation pass the voltage tests of 6.8 | (see Form A.30) | P |
| | i) no leaks of corrosive and harmful substances | | P |
| | ii) enclosure shows no cracks resulting in a hazard | | P |
| | iii) clearances not less than their permitted values | | P |
| | iv) insulation of internal wiring remains undamaged | | P |
| | v) protective barriers not damaged or loosened | | N/A |
| | vi) No moving parts exposed, except permitted by 7.3 | | N/A |
| | vii) no damage which could cause spread of fire | | P |
| 8.2 | Enclosure rigidity test | | P |
| 8.2.1 | Static test | (see Form A.21A) | P |
| | - 30 N with 12 mm rod to each part of enclosure | | P |
| | - in case of doubt test conducted at maximum rated ambient temperature | | P |
| 8.2.2 | Impact test | (see Form A.21A) | N/A |
| | Impact applied to any part of enclosure causing a hazard if damaged | | N/A |
| | Impact energy level and corresponding IK code : | | — |
| | Non-metallic enclosures cooled to minimum rated ambient temperature if below 2 °C | | N/A |
| 8.3 | Drop test | (see Form A.21) | P |
| 8.3.1 | Other than hand-held and direct-plug-in equipment | | N/A |
| | Tests conducted with a drop height or angle of..... : | | — |
| 8.3.2 | hand-held and direct-plug-in equipment | | — |
| | Non-metallic enclosures cooled to minimum rated ambient temperature if below 2 °C | | P |

| | | | |
|-----|---|-----------------|-----|
| | Drop test conducted with an height of 1 m | | P |
| 9 | PROTECTION AGAINST THE SPREAD OF FIRE | | |
| 9.1 | No spread of fire in normal and single fault condition | | P |
| | Mains supplied equipment meets requirements of 9.6 additionally | | P |
| | Conformity is checked by minimum one or a combination of the following (see Figure 11): | (see Form A.22) | — |
| | a) Single Fault test of 4.4; or | (see Form A.1) | P |
| | b) Application of 9.2 (eliminating or reducing the sources of ignition); or | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|----------------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | c) Application of 9.3 (containment of fire within the equipment) | | P |
| 9.2 | Eliminating or reducing the sources of ignition within the equipment | | P |
| | a) 1) Limited-energy circuit (see 9.4); or | | N/A |
| | 2) basic insulation provided for parts of different potential; or | | N/A |
| | Bridging the insulation does not cause ignition | | N/A |
| | b) Surface temperature of liquids and parts (see 9.5) | | N/A |
| | c) No ignition in circuits designed to produce heat | | P |
| 9.3 | Containment of the fire within the equipment, should it occur | | P |
| 9.3.1 | Spread of fire outside equipment reduced to a tolerable level if: | | — |
| | a) Energizing of the equipment is controlled by an operator held switch | | N/A |
| | b) Enclosure is conform with constructional requirements of 9.3.2; and | | P |
| | Requirements of 9.5 are met | | N/A |
| 9.3.2 | Constructional requirements | | — |
| | a) Connectors and insulating material have flammability classification V-2 or better | (see TABLE 1 or Form A.23) | P |
| | b) Insulated wires and cables are flame retardant (VW-1 or equivalent) | (see TABLE:1 or Form A.23) | P |
| | c) Enclosure meets following requirements: | (see Form A.22) | — |
| | 1) Bottom and sides in arc of 5 ° (see Figure 13) to non-limited circuits (9.4) meets: | | — |
| | i) no openings; or | | N/A |
| | ii) perforated as specified in Table 16; or | | N/A |
| | iii) metal screen with a mesh; or | | N/A |
| | iv) baffles as specified in Figure 12 | | N/A |
| | 2) Material of enclosure and any baffle or flame barrier is made of: | | — |
| | Metal (except magnesium); or | | P |
| | Non-metallic materials have flammability classification V-1 or better | (see TABLE 1 or Form A.22) | N/A |
| | 3) Enclosure and any baffle or flame barrier have adequate rigidity | | P |
| 9.4 | Limited-energy circuit | (see Form A.24) | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | a) Potential not more than 30 r.m.s. and 42,4 V peak, or 60 V dc | | N/A |
| | b) Current limited by one of following means: | | — |
| | 1) Inherently or by impedance (see Table 17); or | | N/A |
| | 2) Overcurrent protective device (see Table 18); or | | N/A |
| | 3) A regulating network limits also in single fault condition (see Table 17) | | N/A |
| | c) Is separated by at least basic insulation | | N/A |
| | Fuse or a nonadjustable electromechanical device is used | | N/A |
| 9.5 | Requirements for equipment containing or using flammable liquids | | N/A |
| | Flammable liquids contained in or specified for use with equipment do not cause spread of fire | (see Form A.25) | N/A |
| | Risk is reduced to a tolerable level : | | — |
| | a) The temperature of surface or parts in contact with flammable liquids is 25 °C below fire point | | N/A |
| | b) The quantity of liquid is limited | | N/A |
| | c) Flames are contained within the equipment | | N/A |
| | Detailed instructions for risk-reduction provided | | N/A |
| 9.6 | Over current protection | | P |
| 9.6.1 | Mains supplied equipment protected | | P |
| | Basic insulation between mains parts of opposite polarity provided | | P |
| | Devices not in the protective conductor | | N/A |
| | Fuses or single-pole circuit-breakers not fitted in neutral (multi-phase) | | P |
| 9.6.2 | permanently connected equipment | | — |
| | Overcurrent protection device: | | N/A |
| | Fitted within the equipment; or | | N/A |
| | Specified in manufacturer's instructions | | N/A |
| 9.6.3 | Other equipment | | — |
| | Protection within the equipment | | N/A |
| 10 | EQUIPMENT TEMPERATURE LIMITS AND RESISTANCE TO HEAT | | -- |
| 10.1 | Surface temperature limits for protection against burns | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|------------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Easily touched surfaces within the limits in normal and in single fault condition: | (see Form A.26A) | — |
| | - at an specified ambient temperature of 40 °C | | N/A |
| | - for equipment rated above 40 °C ambient temperature limits not exceeded raised by the difference to 40 °C | | P |
| | Heated surfaces necessary for functional reasons exceeding specified values: | | — |
| | Are recognizable as such by appearance or function; or | | N/A |
| | Are marked with symbol 13 | | N/A |
| | Guards are not removable without tool | | N/A |
| 10.2 | Temperatures of windings | | P |
| | Limits not exceeded in: | (see Form A.26B) | — |
| | normal condition | | P |
| | single fault condition | | P |
| 10.3 | Other temperature measurements | | P |
| | Following measurements conducted if applicable: | (see Form A.26A) | — |
| | a) Value of 60 °C of field-wiring terminal box not exceeded | | N/A |
| | b) Surface of flammable liquids and parts in contact with this liquids | | N/A |
| | c) Surface of non-metallic enclosures | | N/A |
| | d) Parts made of insulating material supporting parts connected to mains supply | | N/A |
| | e) Terminals carrying a current more than 0,5 A | | N/A |
| 10.4 | Conduct of temperature tests | | P |
| 10.4.1 | Tests conducted under reference test conditions and manufacturer's instructions | (see Form A.26A) | P |
| 10.4.2 | Temperature measurement of heating equipment | | N/A |
| | Tests conducted in test corner | (see Form A.26A) | N/A |
| 10.4.3 | Equipment intended for installation in a cabinet or wall | | P |
| | Equipment built in as specified in installation instructions | (see Form A.26A) | P |
| 10.5 | Resistance to heat | | P |
| 10.5.1 | Integrity of clearance and creepage distances | (see Form A.16) | P |
| 10.5.2 | Non-metallic enclosures | | N/A |
| | Within 10 min after treatment: | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| | | | |
|--------|--|-----------------|-----|
| | Equipment subjected to suitable stresses of 8.2 and 8.3 complying with criteria of 8.1 | | N/A |
| 10.5.3 | Insulating material | | P |
| | a) Parts supporting parts connected to mains supply | | P |
| | b) Terminals carrying a current more than 0,5 A | | P |
| | Examination of material data; or | | P |
| | in case of doubt: | | P |
| | 1) Ball pressure test; or | (see Form A.28) | P |
| | 2) Vicat softening test of ISO 306 | | N/A |

| | | | |
|--------|--|--|-----|
| 11 | PROTECTION AGAINST HAZARDS FROM FLUIDS | | |
| 11.1 | Protection to operators and surrounding area provided by equipment | | N/A |
| | All fluids specified by manufacturer considered | | N/A |
| 11.2 | Cleaning | | N/A |
| 11.3 | Spillage | | N/A |
| 11.4 | Overflow | | N/A |
| 11.5 | Battery electrolyte | | N/A |
| | Battery electrolyte leakage presents no hazard | | N/A |
| 11.6 | Specially protected equipment | | N/A |
| 11.7 | Fluid pressure and leakage | | N/A |
| 11.7.1 | Maximum pressure : | | — |
| | Maximum pressure of any part does not exceed Rated | | N/A |
| 11.7.2 | Leakage and rupture at high pressure | | — |
| | Fluid-containing parts subjected to hydraulic test if: | | — |
| | a) product of pressure and volume > 200 kPa; and | | N/A |
| | b) pressure > 50 kPa | | N/A |
| | Parts of refrigerating systems meets pressure-related requirements of IEC 60335-24 or IEC 60335-2-89 | | N/A |
| 11.7.3 | Leakage from low-pressure parts | | N/A |
| 11.7.4 | Overpressure safety device | | N/A |
| | Does not operate in normal use | | N/A |
| | a) Connected as close as possible to parts intended to be protected | | N/A |
| | b) Easy access for inspection, maintenance and repair | | N/A |
| | c) Adjustment only with tool | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | d) No discharge towards person | | N/A |
| | e) No hazard from deposit of discharged material | | N/A |
| | f) Adequate discharge capacity | | N/A |
| | No shut-off valve between overpressure safety device and protected parts | | N/A |

| | | | |
|----------|---|-----------------|-----|
| 12 | Protection against radiation, including laser sources, and against sonic and ultrasonic pressure | | |
| 12.1 | Equipment provides protection | | N/A |
| 12.2 | Equipment producing ionizing radiation | | N/A |
| 12.2.1 | Ionizing radiation | (see Form A.33) | N/A |
| 12.2.1.1 | Equipment meets the following requirements: | | — |
| | a) if intended to emit radiation meets requirements of 12.2.1.2; or | | N/A |
| | tested, classified and marked in accordance to IEC 60405 | | N/A |
| | b) if only emits stray radiation meets requirements of 12.2.1.3 | | N/A |
| 12.2.1.2 | Equipment intended to emit radiation | | — |
| | Effective dose rate of radiation measured : | | — |
| | If dose rate exceeds 5 $\mu\text{Sv/h}$ marked with the following: | | — |
| | a) Symbol 17 (ISO 361) | | N/A |
| | b) Abbreviations of the radionuclides : | | — |
| | c) With maximum dose at 1 m; or : | | — |
| | with dose rate value between 1 $\mu\text{Sv/h}$ and 5 $\mu\text{Sv/h}$ in m : | | — |
| 12.2.1.3 | Equipment not intended to emit radiation | (see Form A.34) | — |
| | Limit for unintended stray radiation of 1 $\mu\text{Sv/h}$ at any easily reached point kept : | | — |
| 12.2.2 | Accelerated electrons | | — |
| | Compartments opened only by the use of a tool | | N/A |
| 12.3 | Ultraviolet (UV) radiation | | N/A |
| | No unintentional hazardous escape of UV radiation: | | — |
| | - checked by inspection; and | | N/A |
| | - evaluation of risk assessment documentation | | N/A |
| 12.4 | Microwave radiation | | N/A |
| | Power density does not exceed 10 W/m^2 : | | N/A |
| 12.5 | Sonic and ultrasonic pressure | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|---|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| 12.5.1 | Sound level | | N/A |
| | No hazardous sound emission | | — |
| | Maximum sound pressure level measured and calculated for maximum sound power level as specified in ISO 3746 or ISO 9614-1 | | N/A |
| | Instruction describes measures for protection | | N/A |
| 12.5.2 | Ultrasonic pressure | | N/A |
| | Equipment not intended to emit ultrasound does not exceed limit of 110 dB between 20 kHz and 100 kHz | | N/A |
| | Equipment intended to emit ultrasound: | | N/A |
| | Outside useful beam does not exceed limit of 110 dB between 20 kHz and 100 kHz | | N/A |
| | If inside useful beam above values exceeded: | | — |
| | Marked with Symbol 14 of table 1 | | N/A |
| | and following information in the documentation: | | — |
| | a) dimensions of useful beam | | N/A |
| | b) area where ultrasonic pressure exceed 110 dB | | N/A |
| | c) maximum sound pressure inside beam area | | N/A |
| 12.6 | Laser sources | | N/A |
| | Equipment meets requirements of IEC 60825-1 | | N/A |

| | | | |
|------|---|--|-----|
| 13 | PROTECTION AGAINST LIBERATED GASES AND SUBSTANCES, EXPLOSION AND IMPLOSION | | |
| 13.1 | Poisonous and injurious gases and substances | | N/A |
| | No poisonous or injurious gases or substances liberated in normal condition | | N/A |
| | Attached data/test reports demonstrate conformity | | N/A |

| | | | |
|--------|---|--|---|
| 13.2 | Explosion and implosion | | P |
| 13.2.1 | Components | | P |
| | Components liable to explode: | | — |
| | Pressure release device provided; or | | P |
| | Apparatus incorporates operator protection (see also 7.7) | | P |
| | Pressure release device: | | — |
| | Discharge without danger | | P |
| | Cannot be obstructed | | P |
| 13.2.2 | Batteries and battery charging | | — |
| | If explosion or fire hazard could occur: | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|---|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Protection incorporated in the equipment; or | | N/A |
| | Instructions specify batteries with built-in protection | | N/A |
| | In case of wrong type of battery used: | | — |
| | No hazard; or | | N/A |
| | Warning by marking and within instructions | | N/A |
| | Equipment with means to charge rechargeable batteries: | | — |
| | Warning against the charging of non-rechargeable batteries; and | | N/A |
| | Type of rechargeable battery indicated; or | | N/A |
| | Symbol 14 used | | N/A |
| | Battery compartment design | | N/A |
| | Single component failure | | N/A |
| | Polarity reversal test | | N/A |
| 13.2.3 | Implosion of cathode ray tubes | | N/A |
| | If maximum face dimensions > 160 mm : | | — |
| | Intrinsically protected and correctly mounted; or | | N/A |
| | enclosure provides protection: | | N/A |
| | If non-intrinsically protected: | | — |
| | Screen not removable without tool | | N/A |
| | If glass screen, not in contact with surface of tube | | N/A |

| | | | |
|--------|---|-----------------|-----|
| 14 | COMPONENTS AND SUBASSEMBLIES | | |
| 14.1 | Where safety is involved, components and subassemblies meet relevant requirements | (see TABLE 1) | P |
| 14.2 | Motors | | N/A |
| 14.2.1 | Motor temperatures | | N/A |
| | Does not present a hazard when stopped or prevented from starting; or | | N/A |
| | Protected by over-temperature or thermal protection device conform with 14.3 | | N/A |
| 14.2.2 | Series excitation motors | | N/A |
| | Connected direct to device, if overspeeding causes a hazard | | N/A |
| 14.3 | Overtemperature protection devices | | P |
| | Devices operating in a single fault condition | (see Form A.38) | P |
| | d) Reliable function is ensured | | P |
| | e) Rated to interrupt maximum current and voltage | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| | | | |
|------|---|----------|-----|
| | f) Does not operate in normal use | | P |
| | If self-resetting device used to prevent a hazard, protected part requires intervention before restarting | | P |
| 14.4 | Fuse holders | | P |
| | No access to hazardous live parts | | P |
| 14.5 | Mains voltage selecting devices | | P |
| | Accidental change not possible | | P |
| 14.6 | Mains transformers tested outside equipment | | N/A |
| 14.7 | Printed circuit boards | | P |
| | Data shows conformity with V-1 of IEC 60695-11-10 or better; or | Min. V-1 | P |
| | Test shows conformity with V-1 of IEC 60695-11-10 or better | | N/A |
| | Not applicable for printed wiring boards with limited-energy circuits (9.4) | | N/A |
| 14.8 | Circuits or components used as transient overvoltage limiting devices | | N/A |
| | Test conducted between each pair of mains supply terminals | | N/A |
| | No hazard resulting from rupture or overheating of the component: | | — |
| | - no bridging of safety relevant insulation | | N/A |
| | - no heat to other parts above the self-ignition points | | N/A |

| | | | |
|------|--|---------------|-----|
| 15 | PROTECTION BY INTERLOCKS | | |
| 15.1 | Interlocks are designed to remove a hazard before operator exposed | No interlocks | N/A |

| | | | |
|------|------------------------------------|--|-----|
| 15.2 | Prevention of reactivation | | N/A |
| 15.3 | Reliability | | N/A |
| | Single fault unlikely to occur; or | | N/A |
| | Cannot cause a hazard | | N/A |

| | | | |
|------|---|--|---|
| 16 | HAZARDS RESULTING FROM APPLICATION | | |
| 16.1 | Reasonably foreseeable misuse | | P |
| | No hazards arising from settings not intended and not described in the instructions | | P |
| | Other cases of reasonably foreseeable misuse addressed by risk assessment | | P |
| 16.2 | Ergonomic aspects | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| | Factors giving rise to a hazard the risk assessment is reflecting those aspects: | | P |
| | a) limitation of body dimensions | | P |
| | b) displays and indicators | | P |
| | c) accessibility and conventions of controls | | P |
| | d) arrangement of terminals | | P |
| 17 | RISK ASSESSMENT | | N/A |
| | Risk assessment conducted, if hazard might arise and not covered by Clauses 6 to 16 | | N/A |
| | Tolerable risk achieved by iterative documented process covering the following: | | — |
| | a) Risk analysis | | N/A |
| | Identifies hazards and estimates risk | | N/A |
| | b) Risk evaluation | | N/A |
| | Plan to judge acceptability of resulting risk level based on the estimated severity and likelihood of a risk | | N/A |
| | c) Risk reduction | | N/A |
| | Initial risk reduced by counter measures; | | N/A |
| | Repeated risk evaluation without new risks introduced | | N/A |
| | Risks remaining after risk assessment addressed in instructions to responsible body: | | — |
| | Information contained how to mitigate these risks | | N/A |
| | Following principles in methods of risk reduction applied by manufacturer in given order: | | — |
| | 1) Risks eliminated or reduced as far as possible | | N/A |
| | 2) Protective measures taken for risks that cannot be eliminated | | N/A |
| | 3) User information about residual risk due to any defect of the protective measures | | N/A |
| | Indication of particular training is required | | N/A |
| | Specification of the need for personal protective equipment | | N/A |
| | Conformity checked by evaluation of the risk assessment documentation | | N/A |
| ANNEX F | ROUTINE TESTS | | N/A |
| | Manufacturer 's declaration | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| IEC 61010-1 | | | |
|-------------|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| ANNEX H | QUALIFICATION OF CONFORMAL COATINGS FOR PROTECTION AGAINST POLLUTION | | |
| H.1 | General | | N/A |
| | Conformal coatings meet the requirements of Clause H.2 and H.3. | | N/A |
| H.2 | Technical properties | | N/A |
| | Technical properties of conformal coatings are suitable for the intended application. In particular: | | — |
| | a) Manufacturer indicate that it is a coating for PWBs; | | N/A |
| | b) rated operating temperature include the temperature range of the indicated application; | | N/A |
| | c) CTI, insulation resistance and dielectric strength are suitable for the intended application; | | N/A |
| | d) Coating have adequate UV resistance, if it is exposed to sunlight; | | N/A |
| | e) Flammability rating of the coating is at least the required flammability rating of the applied PWB. | | N/A |
| H.3 | Qualification of coatings | | N/A |
| | Coating complies with the conformity requirements. | | N/A |
| ANNEX K | INSULATION REQUIREMENTS NOT COVERED BY CLAUSE 6.7 | | P |



| IEC 61010-1 | | | |
|-------------|--------------------|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |

| IEC61010_1P ATTACHMENT | | | |
|---|--|-----------------|---------|
| Clause | Requirement + Test | Result - Remark | Verdict |
| ATTACHMENT TO TEST REPORT IEC 61010-1 EUROPEAN GROUP DIFFERENCES AND NATIONAL DIFFERENCES (Electrical Equipment For Measurement, Control, and Laboratory Use; Part1: General Requirements) | | | |
| Differences according to: EN 61010-1:2010/A1 | | | |
| Attachment Form No.: EU_GD_IEC61010_1P | | | |
| Attachment Originator: TÜV Rheinland LGA Products GmbH | | | |
| Master Attachment: Date 2021-04-12 | | | |
| Copyright © 2021 IEC System for Conformity Testing and Certification of Electrical Equipment (IECEE), Geneva, Switzerland. All rights reserved. | | | |
| | CENELEC COMMON MODIFICATIONS (EN) | | P |
| | Procedure for voltage tests | | P |
| 6.8.3.1 | The a.c. voltage test Replace the first sentence by the following sentence: The voltage tester shall be capable of maintaining the test voltage throughout the test within +/- 5 % of the specified value. | | P |
| Annex ZA (normative) | The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies. | | P |
| Annex ZZ (informative) | Relationship between this European standard and the safety objectives of Directive 2014/35/EU [2014 OJ L96] aimed to be covered | | P |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| 4.4 | TABLE: Testing in SINGLE FAULT CONDITION – Results | | | | Form A.1 | P |
|---|--|-------------------|-----------------|--|----------|-------------|
| Test subclause | Fault No. | Fault description | Td 4.4.3 (NOTE) | How was test terminated | Comments | Meets 4.4.4 |
| 4.4 | 1 | DB1 (S-C) | 10s | After SC, F1 opened. No damage, no hazard. | | Yes |
| | 2 | CE1 (S-C) | 10s | After SC, F1 opened. No damage, no hazard. | | Yes |
| | 3 | T1 (S-C) | 10min | After SC, unit shutdown. No damage, no hazard. | | Yes |
| | 4 | U1 pin4-5 (S-C) | 10min | After SC, unit shutdown. No damage, no hazard. | | Yes |
| NOTE Td = Test duration in hh:mm:ss Record dielectric strength test on Form A.18 and temperature tests on Form A.26A and or A.26 B. Record in the comments column for each test whether carried out during or after SINGLE FAULT CONDITION. | | | | | | |
| Supplementary information: SC: short circuit | | | | | | |

| 5.1.3c) | | TABLE: MAINS supply | | | | Form A.2 | P |
|---|---------|----------------------|---------|--------------|-------|------------------|---|
| | | Marked rating..... : | | 100-240 V | | | — |
| | | Phase..... : | | Single-phase | | | — |
| | | Frequency : | | 50/60 Hz | | | — |
| | | Current : | | 25 A | | | — |
| | | Power : | | 5500 W | | | — |
| | | Power : | | - VA | | | — |
| | | | | | | | |
| Test | Voltage | Frequency | Current | Power | Power | Comments | |
| No. | V | Hz | A | W | VA | | |
| 1 | 100 | 50 | 25.0 | 2500 | -- | Normal operation | |
| 2 | 100 | 60 | 25.0 | 2500 | -- | Normal operation | |
| 3 | 240 | 50 | 25.0 | 6000 | -- | Normal operation | |
| 4 | 240 | 60 | 25.0 | 6000 | -- | Normal operation | |
| NOTE – Measurements are only required for marked ratings. | | | | | | | |
| Supplementary information: | | | | | | | |

| 5.3 | TABLE: Durability of markings | | Form A.3 | P |
|---|-------------------------------|----------------------------|----------|---|
| Marking method (see NOTE) | | Agent | | |
| 1) Adhesive label | | A Water | | |
| 2) Ink printed | | B Isopropyl alcohol | | |
| 3) Laser marked | | C (specify agent) | | |
| 4) Film-coated (plastic foil control panel) | | D (specify agent) | | |
| 5) Imprinted on plastic (moulded in) | | E (specify agent) | | |
| NOTE – Where applicable include print method, label material, ink or paint type, fixing method, adhesive and surface to which marking is fixed. | | | | |
| Marking location | | Marking method (see above) | | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | | | |
|---|----------------------------|-----------------|--------------|--------------|-----------|-----------------|----------|
| 5.1.3c) | TABLE: MAINS supply | | | | | Form A.2 | P |
| | Marked rating..... : | | 100-240 V | | | — | |
| | Phase..... : | | Single-phase | | | — | |
| | Frequency | | 50/60 Hz | | | — | |
| | Current | | 25 A | | | — | |
| | Power | | 5500 W | | | — | |
| | Power | | - VA | | | — | |
| | | | | | | | |
| Test | Voltage | Frequency | Current | Power | Power | Comments | |
| No. | V | Hz | A | W | VA | | |
| Identification (5.1.2) | | | | 1) | | | |
| MAINS supply (5.1.3) | | | | 1) | | | |
| Fuses (5.1.4) | | | | 1) | | | |
| Terminals and operating devices (5.1.5.2) | | | | N/A | | | |
| Switches and circuit breakers (5.1.6) | | | | 1) | | | |
| Double/reinforced equipment (5.1.7) | | | | 1) | | | |
| Field wiring Terminal boxes (5.1.8) | | | | N/A | | | |
| Warning marking (5.2) | | | | 1) | | | |
| Battery charging (13.2.2) | | | | N/A | | | |
| Method | Test agent | Remains legible | Label loose | Curled edges | Comments | | |
| | | Verdict | Verdict | Verdict | | | |
| 1) | A, B | Yes | -- | -- | 30s, pass | | |
| Supplementary information: | | | | | | | |

| | | | | | |
|---|--|----------------------------------|-----------------------------------|-----------------|----------|
| 6.2 | TABLE: List of accessible parts | | | Form A.4 | P |
| 6.1.2 | Exceptions | | | | — |
| 6.2 | Determination of ACCESSIBLE parts | | | | — |
| Item | Description | Determination method (NOTE 5) | Exception under 6.1.2 (NOTE 4) | | |
| 1 | Enclosure | Visual | - | | |
| <p>NOTE 1 – Test fingers and pins are to be applied without force unless a force is specified (see 6.2.2)</p> <p>NOTE 2 – Special consideration should be given to inadequate insulation and high voltage parts (see 6.2)</p> <p>NOTE 3 – Parts are considered to be accessible if they could be touched in the absence of any covering which is not considered to provide suitable insulation (see 6.4).</p> <p>NOTE 4 – Capacitor test may be required (see Form A.5).</p> <p>NOTE 5 – The determination methods are: V = visual; R = rigid test finger; J = jointed test finger; P3 = pin 3 mm diameter; P4 = pin 4 mm diameter.</p> | | | | | |
| Supplementary information: | | | | | |
| 6 | TABLE: Values in normal condition | | | Form A.5 | P |
| 6.1.2 | Exceptions | | 11.2 Cleaning and decontamination | — | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| 6.3.1 | Values in NORMAL CONDITION (see NOTE 1) | | | | | | | 11.3 | Spillage | | | | — |
|----------------|---|--------|--------|-----------------------|-----------|---------|-------------|------|----------|------------------------|----|----|-----------|
| 6.6.2 | Terminals for external circuit | | | | | | | 11.4 | Overflow | | | | — |
| 6.10.3 | Plugs and connections | | | | | | | | | | | | — |
| Item | Voltage | | | Current | | | Capacitance | | | 10 s / 5 s test (NOTE) | | | Comments |
| (see Form A.4) | V r.m.s. | V peak | V d.c. | Test circuit A1/A2/A3 | mA r.m.s. | mA peak | mA d.c. | μC | mJ | V | μC | mJ | |
| 1 | 150 mV | - | - | A1 | 0.35 | - | - | - | - | - | - | - | - |
| 2 | 107 mV | - | - | A1 | 0.25 | - | - | - | - | - | - | - | - |
| 3 | 148 mV | - | - | A1 | 0.33 | - | - | - | - | - | - | - | - |
| 4 | 92 mV | - | - | A1 | 0.24 | - | - | - | - | - | - | - | - |
| 5 | 263 mV | - | - | - | - | - | - | - | - | 0 | - | - | After 10s |
| | | | | | | | | | | | | | |
| | | | | | | | | | | | | | |

NOTE – A 10 s test is specified in 6.1.2 a) b). A. 5 s test is specified in 6.10.3. The capacitance level versus voltage below the limits given from figure 3 of IEC 61010-1.

Supplementary information:

| 6.3.2 | TABLE: Values in single fault condition | | | | | | | | | | | Form A.6 | P |
|---|---|-----------|--------|--------|----------------------|---|------------------------|------------|---------|---------|-----------------|---------------|---|
| Item | Subclause and | Voltage | | | Transient (see NOTE) | | Current | | | | Capacitan ce | Commen ts | |
| (see Form A.4) | fault No. (see Form A.1) | V r.m.s . | V peak | V d.c. | V | s | Test circuit A1/A2/ A3 | mA r.m.s . | mA peak | mA d.c. | μF (see NOTE) | | |
| 1 | 1-4 | 148 mV | - | - | - | - | A1 | 0.34 | - | - | - | - | |
| 2 | 1-4 | 105 mV | - | - | - | - | A1 | 0.23 | - | - | - | - | |
| 3 | 1-4 | 145 mV | - | - | - | - | A1 | 0.31 | - | - | - | - | |
| 4 | 1-4 | 92 mV | - | - | - | - | A1 | 0.23 | - | - | - | - | |
| 5 | 1-4 | - | - | - | - | - | - | - | - | - | - | 0V after 10s. | |
| NOTE – Transient voltages must be below the limits given from Figure 2 and the capacitance below the limits from figure 3 of IEC 61010-1. | | | | | | | | | | | | | |



| 6.3.2 | TABLE: Values in single fault condition | | | | | | | | | | | Form A.6 | P |
|----------------------------|---|-----------|--------|--------|----------------------|---|------------------------|------------|---------|---------|-----------------|--------------|---|
| Item | Subclause and | Voltage | | | Transient (see NOTE) | | Current | | | | Capacitan ce | Commen ts | |
| (see Form A.4) | fault No. (see Form A.1) | V r.m.s . | V peak | V d.c. | V | s | Test circuit A1/A2/ A3 | mA r.m.s . | mA peak | mA d.c. | μF (see NOTE) | | |
| Supplementary information: | | | | | | | | | | | | | |

| | | | | |
|----------------------------------|---|--------------------------------------|----------|---|
| 6.5.2.2 | TABLE: Cross-sectional area of bonding conductors | | Form A.7 | P |
| Conductor location | | CROSS-SECTIONAL AREA mm ² | Verdict | |
| Protect bonding connected to PCB | | 0.75 | Pass | |
| Supplementary information: | | | | |

| 6.5.2.3 | TABLE: Tightening torque test | | Form A.8 | N/A |
|----------------------------|-------------------------------|---------------|-------------------------------|---------|
| Conductor location | | Size of screw | Tightenin g torque [Nm] | Verdict |
| | | | | |
| | | | | |
| Supplementary information: | | | | |

| 6.5.2.4 | TABLE: Bonding impedance of plug connected equipment | | | | Form A.9 | N/A |
|---|--|-------------------|--------------------------------------|---|----------|------------|
| ACCESSIBLE part under test | | Test current A | Voltage attained after 1 min V | Calculated resistance (Maximum 0,1 or 0,2 Ω) [Ω] (NOTE 1) | Verdict | |
| | | | | | | |
| NOTE 1 – For none-detachable power cord the impedance between protective conductor plug pin of MAINS cord and each part shall not exceed 0,2 Ohm. | | | | | | ACCESSIBLE |
| Supplementary information: | | | | | | |

| | | | | | |
|----------------------------|---|-------------------|---|-----------|---------|
| 6.5.2.5 | TABLE: Bonding impedance of permanently connected equipment | | | Form A.10 | N/A |
| ACCESSIBLE part under test | | Test current A | Voltage attained after 1 min (maximum 10 V) V | | Verdict |
| | | | | | |
| Supplementary information: | | | | | |



| | | | | | |
|--|---|---------------------------------|--|--|---------|
| 6.5.2.6 | TABLE: Transformer PROTECTIVE BONDING screen | | | Form A.11 | N/A |
| ACCESSIBLE part under test | | Test current (see NOTE) A | Voltage attained after 1 min (maximum 10 V) V | Calculated resistance (maximum 0,1 Ω) Ω | Verdict |
| | | | | | |
| NOTE – Test current must be twice the value of the overcurrent protection means of the winding. Test is specified in 6.5.2.6 a) or b). | | | | | |
| Supplementary information: | | | | | |

| 6.5.4 | TABLE: protective impedance | | | | | | Form A.12 | N/A |
|---|-----------------------------|----------------------|--------------|------------------------|----------------------|------------------------|-----------|----------|
| A single component | | | | | | | | |
| Component | Location | Measured | | Calculated | Rated | | Verdict | Comments |
| | | Working voltage V | Current A | Power dissipation W | Working voltage V | Power dissipation W | | |
| | | | | | | | | |
| A combination of components | | | | | | | | |
| Component | | | | Location | | | Comments | |
| RESISTORS | | | | R1, R3 | | | | |
| NOTE – A PROTECTIVE IMPEDANCE shall not be a single electronic device that employs electron conduction in a vacuum, gas or semiconductor. | | | | | | | | |
| Supplementary information: | | | | | | | | |

| | | | | | | | |
|----------------------------|---|----------------------|--------------|----------------------|--------------|------------------|----------|
| 6.5.6 | TABLE: Current- or voltage-limiting device | | | | | Form A.13 | N/A |
| Component | Location | Measured | | Rated | | Verdict | Comments |
| | | Working voltage V | Current A | Working voltage V | Current A | | |
| | | | | | | | |
| | | | | | | | |
| | | | | | | | |
| | | | | | | | |
| | | | | | | | |
| Supplementary information: | | | | | | | |

| | | | |
|-----|--|------------------|---|
| 6.7 | TABLE: Insulation requirements- Block diagram of system | Form A.14 | P |
|-----|--|------------------|---|

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | [http:// www.lcs-cert.com](http://www.lcs-cert.com)



| | | | | | | | | | |
|---|--|--|-----------------|--------|--|--------------|---|----------------------------|--|
| 6.7 | TABLE: Insulation requirements- Block diagram of system | | | | | | Form A.14 | P | |
| Pollution degree : 2 | | | | | | | | Overvoltage category | |
| Area | Location | Insulation type | WORKING VOLTAGE | | | Test voltage | Comments (NOTE 3) | | |
| | | (NOTE 1) | RMS V | Peak V | Frequency kHz | (NOTE 2) V | | | |
| A | Primary components live parts to enclosure PE on PCB | BI | 240 | - | -- | 240V | Limit: CAT II 240V: Cl: 2.5, Cr:3.0; Measured: 3.5. | | |
| NOTE 1 – Type of insulation: BI = BASIC INSULATION DI = DOUBLE INSULATION PI = PROTECTIVE IMPEDANCE RI = Reinforced INSULATION SI = Supplementary INSULATION see also Form A.15 for further details | | NOTE 2 - Types of voltage Peak impulse test voltage (pulse) r.m.s. d.c. peak | | | NOTE 3 - OVERVOLTAGE CATEGORIES or POLLUTION DEGREES which differ should be shown under "Comments" | | | | |
| Supplementary Information: | | | | | | | | | |

| | | | | | | | | | | | | | | |
|--|---|-----------------|--------------------------|--------|---------------|-------------|--|-------------|-------------|-----|-----------|----------|---------------------------------------|--|
| 6.7 | TABLE: Insulation requirements- Clearances and Creepages | | | | | | | | | | Form A.15 | P | | |
| 6.2.2 | Examination | | | | | 6.5.4 | Protective impedance | | | | | — | | |
| 6.4.2 | Enclosures and protective barriers | | | | | 6.5.6 | Current- or voltage-limiting device | | | | | — | | |
| 6.4.4 | Impedance | | | | | 9.6.1 | Basic insulation between opposite polarity | | | | | — | | |
| Area | Location | Insulation type | WORKING VOLTAGE (NOTE 2) | | | Clearance | | Creepage | | CTI | Verdict | Comments | | |
| | (See Form A.14) | (NOTE 1) | RMS V | Peak V | Frequency kHz | Required mm | Measured mm | Required mm | Measured mm | | | | | |
| A | Primary components live parts to enclosure on PCB | BI | 240 | - | -- | 2.5 | 3.5 | 3.0 | 3.5 | 175 | P | | | |
| NOTE 1 – refer to Form A.14 for type of insulation shown in the insulation diagram required insulation (see Form A.14) | | | | | | | | | | | | | NOTE 2 – to be used for definition of | |
| Input supply voltage.....: | | V | Hz | | | | | | | | | | | |
| Supplementary information: | | | | | | | | | | | | | | |

| | | | | | | | | | | | | |
|-----|---|--|--|--|--|--|--|--|--|--|-----------|---|
| 6.7 | TABLE: Insulation requirements- Clearances and Creepages | | | | | | | | | | Form A.16 | P |
|-----|---|--|--|--|--|--|--|--|--|--|-----------|---|

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | | | | | | | | | |
|-------|--|---|-----------------|-------------------------|----------------|----------------|----------------|----------------------------|---|-----------|---------|----------|-------------------|
| 6.4.2 | | ENCLOSURES or PROTECTIVE BARRIERS | | | | | | 9.6.1 | Overcurrent protection basic insulation between MAINS parts | | — | | |
| 8 | | Mechanical resistance to shock and impact | | | | | | 10.5.1 | Integrity of CLEARANCES and CREEPAGE distances | | — | | |
| Area | Location | | Insulation type | Mechanical tests (NOTE) | | | | Test at max. | Measured after test (if required) | | Verdict | Comments | |
| | (See Form A.14) | | | Applied force | Rigidity (8.2) | | Drop (8.3) | | RATED ambient | Clearance | | | Creepage distance |
| | | | | N | Static (8.2.1) | Impact (8.2.2) | Normal (8.3.1) | Hand-held/Plug-in (10.5.1) | mm | mm | | | |
| A | Primary components live parts to enclosure | | BI | Yes | 30N | 1m | N/A | N/A | 40 | 3.5 | 3.5 | P | |

NOTE – Refer to Form A.18 for dielectric strength tests following the above tests.

Supplementary information:

| | | | |
|-----------|---|-----------|-----|
| 6.7.2.2.2 | TABLE: Reliability of potted components | Form A.17 | N/A |
| 14.1 b) | Components and subassemblies | | N/A |

| Temperature Cycling Test | | | | | | | |
|------------------------------------|------|----|--|---------------|-------------|----------------------------|-------------|
| Manufacturer | | | | | | | |
| Type | | | | | | | |
| Construction | | | | | | | |
| Potting compound | | | | | | | |
| CREEPAGE distances measured | | | | | | | |
| CLEARANCES measured | | | | | | | |
| Thickness through insulation | | | | | | | |
| Adhesive test Pass/Fail..... | | | | | | | |
| Test temperature T °C | | | | | | | |
| Cycles at U= AC 500 V | | | | | | Leakage current (500 V) Ma | |
| Number of cycles | Date | | | 68 h / 125 °C | 1 h / 25 °C | 2 h / 0 °C | 1 h / 25 °C |
| 1. Cycle from | | to | | | | | |
| 2. Cycle from | | to | | | | | |
| 3. Cycle from | | to | | | | | |
| 4. Cycle from | | to | | | | | |
| 5. Cycle from | | to | | | | | |
| 6. Cycle from | | to | | | | | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | | | |
|---|--|----|--|----------------------|--|---------|--|
| 7. Cycle from | | to | | | | | |
| 8. Cycle from | | to | | | | | |
| 9. Cycle from | | to | | | | | |
| 10. Cycle from | | to | | | | | |
| After Cycling Test : | | | | | | | |
| Humidity conditioning | | | | 48 h | | | |
| Requirements for dielectric strength (s. insulation diagram) | | | | Test voltage V r.m.s | | Verdict | |
| Basic insulation _____ V r.m.s. | | | | | | | |
| Supplementary insulation _____ V r.m.s. | | | | | | | |
| Reinforced insulation _____ V r.m.s. | | | | | | | |
| NOTE – to be used for evaluation of components containing insulation through solid insulation, when the component standard require thermal cycling test. Ref Clause 14.1 and Figure 15, option b) | | | | | | | |
| Supplementary information: | | | | | | | |

| | | | | | | | |
|---|--|-----------------|-------------------|-------------------------------|-----------------|------------------|----------|
| 6.8 | TABLE: Dielectric strength tests | | | | | Form A.18 | P |
| 4.4.4.1 b) | Conformity after application of SINGLE FAULT CONDITIONS ¹ | | | | | | P |
| 6.4 | Primary means of protection ² | | | | | | P |
| 6.6 | Connections to external circuits | | | | | | P |
| 6.7. | Insulation requirements ² (see Annex K) | | | | | | P |
| 6.10.2 | Fitting of non-detachable MAINS supply cords ¹ | | | | | | N/A |
| 9.2 a) 2) | Eliminating or reducing the sources of ignition within the equipment | | | | | | N/A |
| 9.4 c) | Limited-energy circuit | | | | | | N/A |
| 9.6.1 | Overcurrent protection basic insulation between MAINS – parts | | | | | | N/A |
| | Test site altitude..... | | | 500 m | | — | |
| | Test voltage correction factor (see table 10)..... | | | 1.12 | | — | |
| Location or references from Forms A.1 and A.14 | Clause or sub-clause | Humidity Yes/No | Working voltage V | Test voltage r.m.s./peak/d.c. | Comments (NOTE) | Verdict | |
| | | | | | | | |
| | | | | | | | |
| | | | | | | | |
| | | | | | | | |
| ¹ Record the fault, test or treatment applied before the dielectric strength test. ² Humidity preconditioning required. | | | | | | | |
| NOTE: Test duration may be recorded. | | | | | | | |
| Supplementary information: | | | | | | | |

| | | | | | | | |
|---------------|------------------------------|--------|---------|-----------|---------|------------------|------------|
| 6.10.2 | TABLE: Cord anchorage | | | | | Form A.19 | N/A |
| Location | Mass kg | Pull N | Verdict | Torque Nm | Verdict | Comment | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | | | |
|--|-----------------------|------------|-----------|----------|--------------|-----------|---------|
| 6.10.2 | TABLE: Cord anchorage | | | | | Form A.19 | N/A |
| Location | | Mass kg | Pull N | Verdict | Torque Nm | Verdict | Comment |
| | | | | | | | |
| Dielectric strength test for 1 min. (6.8.3.1)..... : | | | | V r.m.s. | | | |
| Supplementary information: | | | | | | | |

| | | | | | | | | | | | | | | | |
|----------------------------|--|--|-------------------|-------------|------------|-------------|-----------|------------|-------------|--------------|-------------------|------------|-------------|----------|--|
| 7. | TABLE: Protection against mechanical HAZARDS | | | | | | | | | | | | Form A.20 | N/A | |
| 7.3.4 | Limitation of force and pressure | | | | | | | | | | | | | — | |
| 7.3.5 | Gap limitations between moving parts | | | | | | | | | | | | | — | |
| Part / Location | Clause 7.3.4 | | Clause 7.3.5.1 | | | | | | | | Clause 7.3.5.2 | | Verdict | Comments | |
| | Continuous | Temporary | Minimum gaps [mm] | | | | | | | | Maximum gaps [mm] | | | | |
| | Contact pressure max. 50 N /cm² @ max. 150 N | max. 250 N / 3 cm² @ max. 0,75 s | Torso 500 | Head 300 | Leg 180 | Foot 120 | Toe 50 | Arm 120 | Hand 100 | Finger 25 | Head 120 | Foot 35 | Finger 4 | | |
| | | | | | | | | | | | | | | | |
| Supplementary information: | | | | | | | | | | | | | | | |

| | | | | |
|---------------------------------------|---|-----------------------|-----|---------|
| 8.2 | ENCLOSURE rigidity test | Form A.21A | | P |
| 8.2.1 | Static test | | | P |
| | Material of enclosure : | Non-Metal | | — |
| | Preparation for the test: | - | | — |
| | Operated at ambient temperature : | - ° C | - h | — |
| Location | | Comments | | Verdict |
| 1) Enclosure | | 30N force. No damage. | | P |
| | | | | |
| | | | | |
| Supplementary information: For sender | | | | |
| 8.2.2 | Dynamic test | | | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | |
|----------------------------|-------------------------------|----------|---------|
| | Material of enclosure | Metal | — |
| | Corresponding IK-code | | — |
| | Preparation for the test: | -- | — |
| | Cooled to (temperature) | -- ° C | — |
| Location | | Comments | Verdict |
| | | | |
| Supplementary information: | | | |

| | | | |
|---------------------------------------|--|-------------------|----------|
| 8.3 | Drop test | Form A.21B | P |
| 8.3.1 | Other equipment | | N/A |
| | Location | Raised up to | Comments |
| | -- | 500mm 30 ° | — |
| | | | |
| Supplementary information: For sender | | | |
| 8.3.2 | Hand-held EQUIPMENT and direct plug-in equipment | | P |
| | Material of enclosure | non-metallic | — |
| | Preparation for the test: | 10mins | — |
| | Cooled to (temperature) | 24.5 | — |
| | Location | Comments | Verdict |
| | 1) Side | No damage | P |
| | 2) Edge | No damage | P |
| | 3) Corner | No damage | P |
| Supplementary information: | | | |

| | | | | | |
|----------------------------|--|-----------------------------------|---------------------------|-----------|---|
| 9 | TABLE: Protection against the spread of fire | | | Form A.22 | P |
| Item | Source of HAZARD or area of the equipment considered (circuit, component, liquid etc.) | Protection Method (9.1 a, b or c) | Protection details | Verdict | |
| 1 | Internal circuits | 9a | See form A.1 for details. | P | |
| 2 | Internal circuits | 9c | See form A.1 for details. | P | |
| Supplementary information: | | | | | |

| | | | |
|---------------------------------|---|------------------|----------|
| 9.3.2 | TABLE: Constructional requirements | Form A.23 | P |
| 14.7 | Printed circuit boards | | P |
| No test need, PCB V-1 or better | | | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | | | | |
|--|-----------|--------|---|---|---|---|---|---|
| Material tested.....: | | | | | | | | — |
| Generic name.....: | | | | | | | | — |
| Material manufacturer | | | | | | | | — |
| | | | | | | | | |
| Type | | | | | | | | — |
| Colour.....: | | | | | | | | — |
| Conditioning details.....: | | | | | | | | — |
| | | | | | | | | |
| | | Sample | | | | | | |
| | | 1 | 2 | 3 | 4 | 5 | 6 | |
| Thickness of specimen | mm | | | | | | | |
| Duration of flaming after first Application | s | | | | | | | |
| Duration of flaming plus glowing After second application | s | | | | | | | |
| Specimen burns to holding clamp | Yes/No | | | | | | | |
| Cotton ignited | Yes/No | | | | | | | |
| Sample result | Pass/Fail | | | | | | | |
| Supplementary information: | | | | | | | | |

| | | | | | | | |
|--|---|-----------------------------------|--|-----------------------|----------|------------------|------------|
| 9.4 | TABLE: Limited-energy circuit | | | | | Form A.24 | N/A |
| Item | 9.4 a) | 9.4 b) Current limitation (NOTE) | | 9.4 c) | Decision | Comments | |
| or Location (see Form A.22) | Maximum potential in circuit voltage r.m.s./d.c. V | Maximum available current A | Overload protection after 120 s A | Circuit separation | Yes/No | | |
| | | | | | | | |
| NOTE – Maximum values see Tables 17 and 18. of 61010-1 | | | | | | | |
| Supplementary information: | | | | | | | |

| | | | | | |
|----------------------------|--|-----------------------|----------------|------------------|------------|
| 9.5 | TABLE: Requirements for equipment containing or using flammable liquids | | | Form A.25 | N/A |
| Type of liquid | | 9.5 Flammable liquids | | | Verdict |
| | | b) Quantity | c) Containment | | |
| | | | | | |
| Supplementary information: | | | | | |



| | | | | | | |
|--|---|--------------------------|---------------------------------------|----------------------------|-------------------|----------|
| 10. | TABLE : Temperature Measurements | | | | Form A.26A | P |
| 10.1 | Surface temperature limits – NORMAL CONDITION and / or SINGLE FAULT CONDITION | | | | | N/A |
| 10.2 | Temperature of windings- NORMAL CONDITION and / or SINGLE FAULT CONDITION | | | | | N/A |
| 10.3 | Other temperature measurements | | | | | P |
| Operating conditions: | | Normal operation | | | | |
| Frequency | | 60 Hz | Test room ambient temperature (ta)... | | 55.0 °C | |
| Voltage | | 240 V | Test duration..... | | 01 h 36 min | |
| Part / Location | | t_m °C (measure) | t_c °C (K+40) | t_{max} °C (limit) | Verdict | Comments |
| Terminal | | 73.6 | -- | 85 | P | |
| Terminal support | | 66.9 | -- | 85 | P | |
| Power supply | | 79.6 | -- | 105 | P | |
| Relay | | 82.3 | -- | 85 | P | |
| RV1 | | 86.3 | -- | 85 | P | |
| C1 body | | 82.4 | -- | 105 | P | |
| PCB near U1 | | 87.3 | -- | 130 | P | |
| T1 winding | | 86.5 | -- | 110 | P | |
| T1 bobbin | | 81.4 | | 110 | | |
| RV1 (control board) | | 82.3 | -- | 85 | P | |
| CX1 body (control board) | | 80.6 | -- | 110 | P | |
| CE1 body (control board) | | 78.6 | -- | 105 | P | |
| CY1 body (control board) | | 77.4 | -- | 125 | P | |
| PCB near DB1 (control board) | | 85.6 | -- | 130 | P | |
| PCB near U1 (control board) | | 86.9 | -- | 130 | P | |
| Enclosure inside | | 68.7 | -- | Ref. | P | |
| Enclosure outside | | 60.4 | -- | 65 | P | |
| Ambient | | 55.0 | -- | -- | -- | |
| <p>NOTE 1 - t_m = measured temperature t_c = t_m corrected ($t_m - t_a + 40$ °C or max. RATED ambient) t_{max} = maximum permitted temperature</p> <p>NOTE 2 - see also 14.1 with reference to component operating conditions</p> <p>NOTE 3 - Record values for NORMAL CONDITION and / or SINGLE FAULT CONDITION in this Form use additional form if necessary</p> <p>NOTE 4 - see Form A.26B for details of winding temperature measurements</p> | | | | | | |
| Supplementary information: | | | | | | |

| | | | |
|-------------|---|-------------------|------------|
| 10.2 | TABLE: Temperature of windings | Form A.26B | N/A |
| | Resistance method Temperature Measurements | | |
| 4.4.2.7 | MAINS transformers | | |
| 14.2.1 | Motor temperatures | | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | | | | |
|---------------------------|------------|---|--------------|---------|----------|------------------------|---------|----------|
| Operating conditions ...: | | | | | | | | |
| Frequency | Hz | Test room ambient temperature (ta1/ta2) ..: | | | | / °C (initial / final) | | |
| Voltage | V | Test duration | | | | h min | | |
| Part / Designation | Rcold Ω | Rwarm Ω | Current A | tr K | tc °C | tmax °C | Verdict | Comments |
| | | | | | | | | |

NOTE 1- R_{cold} = initial resistance
 t_r = temperature rise
 t_{max} = maximum permitted temperature
 R_{warm} = final resistance
 $t_c = t_r$ corrected ($t_c = t_r - \{t_{a2} - t_{a1}\} + [40\text{ °C or max RATED ambient}]$)
NOTE 2 - Indicate insulation class (IEC 60085) under comments (optional)
NOTE 3 - Record values for NORMAL CONDITION and / or SINGLE FAULT CONDITION in this Form use additional form if necessary

Supplementary information:

| | | | | | | |
|---------------|---|--------------------------------------|--|--|------------------|---------|
| 10.5.2 | TABLE: Resistance to heat of non-metallic ENCLOSURES | | | | Form A.27 | N/A |
| | Test method used: a) | | | | | — |
| | Non operative treatment..... : [] | | | | | N/A |
| | Empty ENCLOSURE : [] | | | | | N/A |
| | Operative treatment..... : [] | | | | | N/A |
| | Temperature during tests : | | | | | — |
| Description | | Material | | | Comments | Verdict |
| | | | | | | |
| | | | | | | |
| | | | | | | |
| | | | | | | |
| | | Dielectric strength test (6.8) | | | V r.m.s. | N/A |

NOTE – Within 10 minutes of the end of treatment suitable tests in acc. to 8.2 and 8.3 must be conducted and pass criteria of 8.1.

Supplementary information:

| | | | | | |
|----------------------------|---|------------------------|--|-----------------------------|---------|
| 10.5.3 | TABLE: Insulating Materials | | | Form A.28 | P |
| 10.5.3 1) | Ball-pressure test | | | | P |
| | Max. allowed impression diameter : 2 mm | | | | — |
| Part | | Test temperature °C | | Impression Diameter (mm) | Verdict |
| PCB | | 125 | | 0.6 | P |
| Terminal support | | 125 | | 0.8 | P |
| Enclosure | | 75 | | 1.0 | P |
| Transformer bobbin | | 125 | | 0.6 | P |
| Supplementary information: | | | | | |
| 10.5.3 2) | Vicat softening test (ISO 306) | | | Form A.29 | N/A |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| | | | | | |
|----------------------------|--|--------------------------------|------|--------------------------|---------|
| 10.5.3 | TABLE: Insulating Materials | | | Form A.28 | P |
| 10.5.3 1) | Ball-pressure test | | | | P |
| | Max. allowed impression diameter : | | 2 mm | | — |
| Part | | Vicat softening temperature °C | | Thickness of sample (mm) | Verdict |
| | | | | | |
| Supplementary information: | | | | | |

| | | | | | | | | | | | | |
|--|--|-----------------|----------------|------------------|-----------------|-----------------|-----------------|-------------------|-------------------|----------------|-----------|----------|
| 8 | TABLE: Mechanical resistance to shock and impact | | | | | | | | | | Form A.30 | P |
| 11 | Protection against HAZARDS from fluids | | | | | | | | | | P | |
| Voltage tests can be carried out once after performing the tests of clause 8 and clause 11. However, if voltage tests are carried out separately after each set of tests, two forms can be used. | | | | | | | | | | | | |
| | Clause 8 tests | | | | Clause 11 tests | | | | | | | |
| Location (see Form A.14) | Static (8.2.1) 30 N | Impact (8.2.2) | Normal (8.3.1) | Handheld Plug-in | Cleaning (11.2) | Spillage (11.3) | Overflow (11.4) | IEC 60529 (11.6) | Working voltage V | Test voltage V | Verdict | Comments |
| Enclosure top | Yes | 1m | - | - | - | - | - | - | 3 | 3000 VAC | P | |
| Enclosure bottom | Yes | 1m | - | - | - | - | - | - | 3 | 3000 VAC | P | |
| Enclosure side | Yes | 1m | - | - | - | - | - | - | 3 | 3000 VAC | P | |
| NOTE – Use r.m.s., d.c. or peak to indicate the used test voltage. | | | | | | | | | | | | |
| Supplementary information: | | | | | | | | | | | | |

| | | | | | | | |
|---|---|-------------------|------------------|----------------------|----------------|-----------|-----|
| 11.7.2 | TABLE: Leakage and rupture at high pressure | | | | | Form A.31 | N/A |
| Part | Maximum permissible working pressure Mpa | Test pressure MPa | Leakage Yes / No | Deformation Yes / No | Burst Yes / No | Comments | |
| | | | | | | | |
| NOTE – see also Annex G with requirements for USA and Canada. | | | | | | | |
| Supplementary information: | | | | | | | |

| | | | | | |
|------------------|--------------------------------------|-----------------------|---------|------------------|-----|
| 12.2.1 | TABLE: Ionizing radiation | | | Form A.33 | N/A |
| 12.2.1.2 | Equipment intended to emit radiation | | | | |
| Locations tested | | Measured values µSv/h | Verdict | Comments | |
| | | | | | |
| | | | | | |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| | | | | | |
|----------------------------|--|--------------------------|---------|------------------|-----|
| 12.2.1 | TABLE: Ionizing radiation | | | Form A.33 | N/A |
| 12.2.1.2 | Equipment intended to emit radiation | | | | |
| Locations tested | | Measured values μSv/h | Verdict | Comments | |
| Supplementary information: | | | | | |
| 12.2.1.3 | Equipment not intended to emit radiation | | | Form A.34 | N/A |
| | Max. allowed effective dose rate at 100 mm.....: | | 1 μSv/h | — | |
| Locations tested | | Measured values μSv/h | Verdict | Comments | |
| | | | | | |
| Supplementary information: | | | | | |

| | | | | | |
|---|---------------------------|--|--------------------------------------|------------------|-----|
| 12.5.1 | TABLE: Sound level | | | Form A.35 | N/A |
| Locations tested | | Measured maximum sound pressure level Db(A) | Calculated maximum sound power level | | |
| At operator's normal position and at bystanders' positions | | | | | |
| a) | | | | | |
| b) | | | | | |
| c) | | | | | |
| d) | | | | | |
| e) | | | | | |
| f) | | | | | |
| Supplementary information: | | | | | |
| 12.5.2 | Ultrasonic pressure | | | Form A.36 | N/A |
| Locations tested | | Measured values | | Comments | |
| | | dB | kHz | | |
| At operator's normal position | | | | | |
| At 1 m from the ENCLOSURE | | | | | |
| a) | | | | | |
| b) | | | | | |
| c) | | | | | |
| d) | | | | | |
| e) | | | | | |
| NOTE – No limit is specified at present, but a limit of 110 dB above the reference pressure value of 20 μPa is under consideration for applicable frequencies between 20 kHz and 100 kHz. | | | | | |



| | | | |
|----------------------------|---|--------------------------------------|-----|
| 12.5.1 | TABLE: Sound level | Form A.35 | N/A |
| Locations tested | Measured maximum sound pressure level Db(A) | Calculated maximum sound power level | |
| Supplementary information: | | | |

| | | | |
|----------------------------|--|------------------|---------------|
| 13.2.2 | TABLE: Batteries | Form A.37 | N/A |
| | Battery load and charging circuit diagram: | | |
| | Battery type | | — |
| | Battery manufacturer/model/catalogue No..... | | — |
| | Battery ratings | | — |
| | Reverse polarity instalment test | | N/A |
| Single component failures | | Verdict | |
| Component | | Open circuit | Short circuit |
| | | | |
| | | | |
| | | | |
| Supplementary information: | | | |

| | | | |
|--|---|------------------|----------|
| 14.3 | TABLE: Over temperature protection devices | Form A.38 | N/A |
| Reliability test | | | |
| Component | Type (NOTE) | Verdict | Comments |
| | | | |
| | | | |
| NOTE: NSR = non-self-resetting (10 times) NR = non-resetting (1 time) SR = self-resetting (200 times) | | | |
| Supplementary information: | | | |

| | | | |
|--------------------|---|------------------|-----|
| 4.4.2.7 | TABLE: MAINS transformer | Form A.39 | N/A |
| 4.4.2.7.2 | Short circuit | | N/A |
| 14.6 | MAINS transformers tested outside equipment | | N/A |
| Type | / | | — |
| Manufacturer | / | | — |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http://www.lcs-cert.com



| | | | | | | |
|--|--|---|--|--|------------------|-----|
| 4.4.2.7 | TABLE: MAINS transformer | | | | Form A.40 | N/A |
| 4.4.2.7.3 | Overload tests (for MAINS transformers) | | | | | |
| 14.6 | MAINS transformers tested outside equipment | | | | | |
| Elapsed time | | | | | | |
| Current, A primary | | | | | | |
| secondary | | | | | | |
| Winding temperature, °C primary | | | | | | |
| (see NOTE 2) secondary | | | | | | |
| Tissue paper / cheesecloth OK ? (Pass / Fail) | | | | | | |
| Voltage tests (see NOTE 3) | | | | | | |
| Primary to secondary | NB | | | | | |
| Primary to core | NB | | | | | |
| Secondary to core | NB | | | | | |
| Verdict | | P | | | | |
| NOTE 1: | Primary fuse - PF / () A Secondary fuse - SF / () A Overtemperature protection - OP / () °C Impedance protection - Z Indicate method of measurement TC = with thermocouple R = resistance method | | | | | |
| NOTE 2: | If resistance method is used, record resistance in cold and warm condition in FormA.26B! | | | | | |
| NOTE 3: | Record the voltage applied and the type of voltage (r.m.s. / d.c. / peak) and for results use NB = no breakdown or B = breakdown | | | | | |
| Supplementary information: | | | | | | |

| 14.8 | TABLE: Transient overvoltage limiting devices | | | | | | | | Form A.41 | N/A |
|---|--|---------------------|----------------|----------|----------|--------------|------------------|-------------------------|------------------|----------|
| Component / Designation | Overvoltage Category | MAINS voltage V rms | Test voltage V | t_m °C | t_c °C | t_{max} °C | Rupture Yes / No | Circuit breaker tripped | Verdict | Comments |
| | | | | | | | | | | |
| Test room ambient temperature | | °C | | | | | | | | |
| NOTE - t_m = measured temperature $t_c = t_m$ corrected ($t_m - t_a + 40$ °C or max. RATED ambient) t_{max} = maximum permitted temperature Conformity is checked by applying 5 positive and 5 negative impulses with the applicable impulse withstand voltage, spaced up to 1 min apart, from a hybrid impulse generator (see IEC 61180-1). | | | | | | | | | | |
| Supplementary information: | | | | | | | | | | |

| | | | |
|----------------|---|------------------|-----|
| Annex H | TABLE: Qualification of conformal coating for protection against pollution | Form A.42 | N/A |
|----------------|---|------------------|-----|

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| Technical properties | | | | | | | | | | | |
|--|-----------------------|-----------|---------|------------|---|---|---|---|---|---------|----------|
| Manufacturer | | | | | | | | | | — | |
| Type | | | | | | | | | | — | |
| Meet requirements of ANSI / UL 746E | | | | [yes / no] | | | | | | | |
| Manufacturer declaration of coating material : | | | | [yes / no] | | | | | | | |
| Operating temperature of coating | | | | [] °C | | | | | | | |
| Comparative tracking index (CTI) | | | | [] | | | | | | | |
| Insulation resistance | | | | [] Ω | | | | | | | |
| Dielectric strength | | | | [] V | | | | | | | |
| UV resistance (if required) | | | | [yes / no] | | | | | | | |
| Flammability rating | | | | | | | | | | | |
| Preparation of the test specimens conducted: | | | | [yes / no] | | | | | | | |
| Item | Test conditioning | Parameter | Td h | Samples | | | | | | Verdict | Comments |
| | | | | 1 | 2 | 3 | 4 | 5 | 6 | | |
| 1 | Scratch resistance | | | | | | | | | | |
| | Visual inspection | | | | | | | | | | |
| 2 | Cold | | 24 | | | | | | | | |
| 3 | Dry heat | | 48 | | | | | | | | |
| 4 | Rapid temp. change | | | | | | | | | | |
| 5 | Damp heat | | 24 | | | | | | | | |
| 6 | Adhesion of coating | 5 N | | | | | | | | | |
| | Visual inspection | | | | | | | | | | |
| 7 | Humidity | | 48 | | | | | | | | |
| 8 | Insulation resistance | >= 100 Ω | | | | | | | | | |
| | Visual inspection | | | | | | | | | | |
| | | | | | | | | | | | |
| NOTE Td = Test duration time | | | | | | | | | | | |
| Supplementary information: | | | | | | | | | | | |



| TABLE 1: - List of components and circuits relied on for safety | | | | | P |
|---|--|----------------------|----------------------------------|-----------------|-------------------------|
| Object / part No | Manufacturer / trademark (NOTE 1) | Type / model | Technical data (NOTE 2) | Standard | Mark(s) of conformity1) |
| Plastic enclosure | Shenzhen Jinhengguan Technology Co., Ltd. | 940(f1) | V-0, 80°C | UL 94 | UL E121562 |
| PCB | Dongguan Bestchoice Electronics co., Ltd. | YX-11 | V-0, Min.130°C | UL 796 | UL E302201 |
| (Alt.) | SHENZHEN QUNHUI ELECTRONICS CO LTD | QH-D | V-0, Min.130°C | UL 796 UL 94 | UL E506706 |
| Varistor (RV1 power supply board) | SHANTOU HIGH-NEW ZONE SONGTIAN ENTERPRISE CO., LTD | STE-10D471KBS | Min.300V 85°C | EN 61051 | VDE 40023049 |
| (Alt.) | SHENZHEN SOCAY ELECTRONICS CORP LTD. | 10D471KJ | Min.300V 85°C | EN 61051 | VDE 40049027 |
| Varistor (RV1 Main control board) | SHENZHEN SOCAY ELECTRONICS CORP LTD. | 10D511K | Min.320V -40~105°C | EN 61051 | VDE 40049027 |
| Fuse (F1) | Dongguan REOMAX Electronics corp.,Ltd. | MTS1100A | T1A, 250V | EN 60127 | VDE 40039420 |
| E-Capacitor (CE1, CE2) | DONG GUAN KNSCHA ELECTRONICS CO., LTD. | D8L12 | -40~+105°C 400V 6.8uF | EN 60730-1 | Test with appliance |
| (Alt.) | Shenzhen huarong weiyee electronics co., Ltd. | D8L12 | -40~+105°C 400V M 6.8uF 2000H | EN 60730-1 | Test with appliance |
| Y-Capacitor (CY1) | SHANTOU HIGH-NEW ZONE SONGTIAN ENTERPRISE CO., LTD | Y5P | 10mm Y5P 400V K 220pF | EN60384-14 | VDE 40025754 |
| (Alt.) | Hongzhi Enterprises Ltd. | Y1-B-221K | 400V K 220pF | EN60384-14 | VDE 40038760 |
| Relay | Dongguan Golden Electrical Appliance Co Ltd | GK-A-1B-5D | DC5V 30A 250VAC | EN 61810-1 | TUV R50163611 |
| X-Capacitor (CX1) | SURETOP TECHNOLOGY Co.Ltd. | SET-X2-473K275VB3L20 | 7.5mm AC275V K 0.047uF | EN60384-14 | VDE 400345085 |
| Internal wire for input | ShenZhen Jinfengsheng Electronic Co., Ltd. | 12AWG | 105°C,300V,12AWG | UL 758 | Test with appliance |

TRF No. IEC61010_1P

Shenzhen LCS Compliance Testing Laboratory Ltd.

Add: Room 101, 201, Building A and Room 301, Building C, Juji Industrial Park, Yabianxueziwei, Shajing Street, Bao'an District, Shenzhen, Guangdong, China

Tel: +(86) 0755-8259 1330 | Fax: +(86) 0755-8259 1332 | E-mail: webmaster@lcs-cert.com | http:// www.lcs-cert.com



| TABLE 1: - List of components and circuits relied on for safety | | | | | P |
|---|--|-------------------------|--------------------------|------------|-------------------------|
| Object / part No | Manufacturer / trademark (NOTE 1) | Type / model | Technical data (NOTE 2) | Standard | Mark(s) of conformity1) |
| Internal wire for connect to control board | ShenZhen Jinfengsheng Electronic Co., Ltd. | 22AWG | 80°C,300V,22AWG | UL 758 | Test with appliance |
| Terminal | Dongguan Changhe Electronics Co., Ltd. | CA350-04-500-3P-04B-02E | 250V 10A 500mm | EN 60730-1 | Test with appliance |
| Plastic material near terminal | Shenzhen Jinhengguan Technology Co., Ltd. | 940(f1) | V-0, 80°C | UL 94 | UL E121562 |
| Terminal block | Dongguan Changhe Electronics Co.,Ltd. | CA350-04-500-3P-04B-02E | 250V, Max.10A, Max.125°C | EN 60998-1 | VDE 40021481 |
| Transformer (T1) | Shenzhen Xinchuang Long Electronic Technology Co., Ltd | EE10 | 2.8mH 5V/500mA | \ | Test with appliance |
| <p>NOTE → 1 List all different manufacturers of the above components → 2 May include electrical, mechanical values → 3 List licence no or method of acceptance</p> <p>→ 4 asterisk indicates mark assuring agreed level of surveillance s</p> | | | | | |



ATTACHMENT 1

Photo Documentation

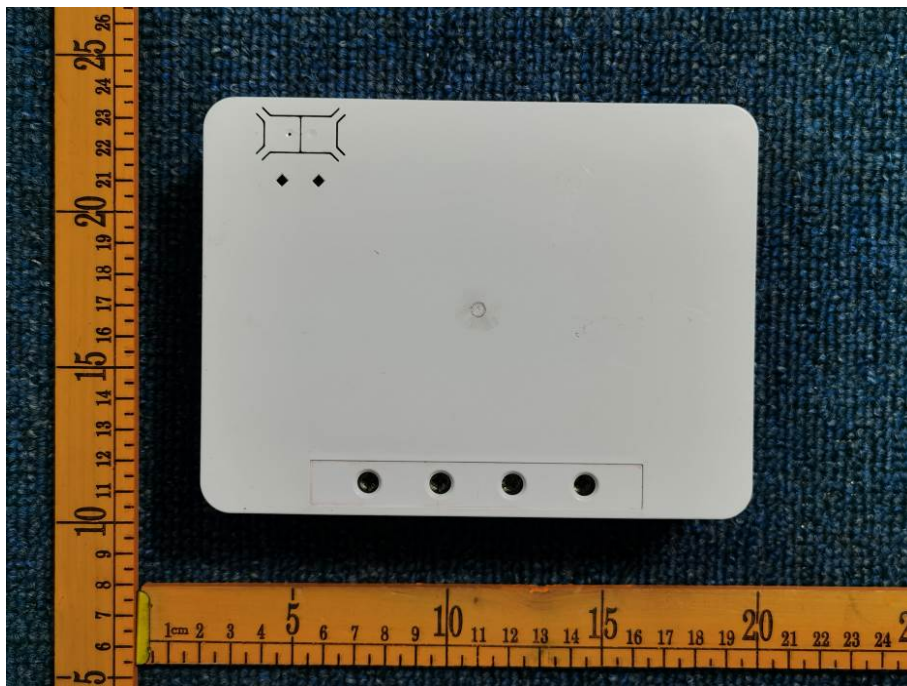


Figure 1 External View

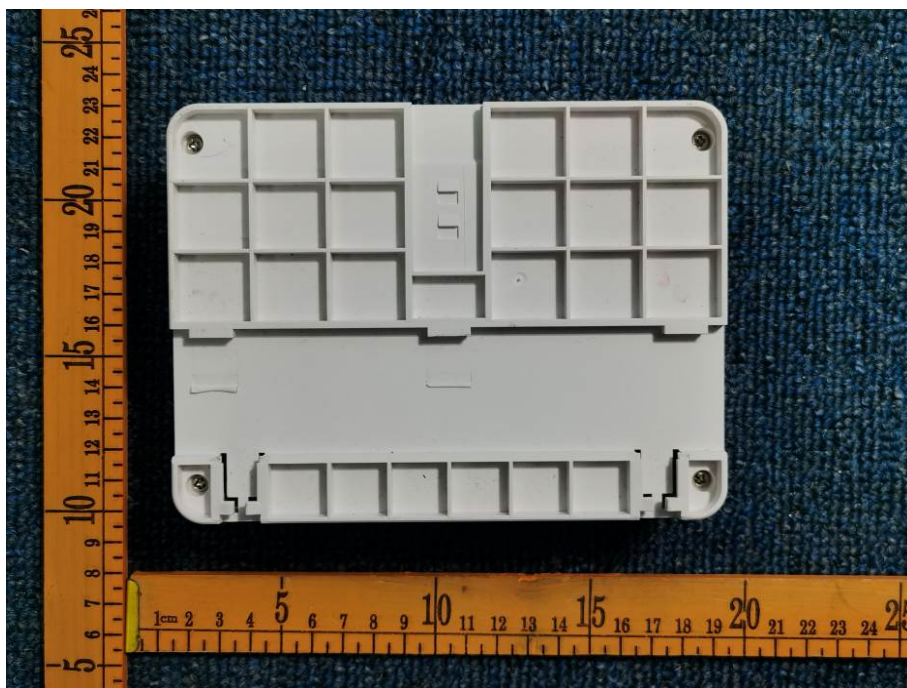


Figure 2 External View



ATTACHMENT 1

Photo Documentation

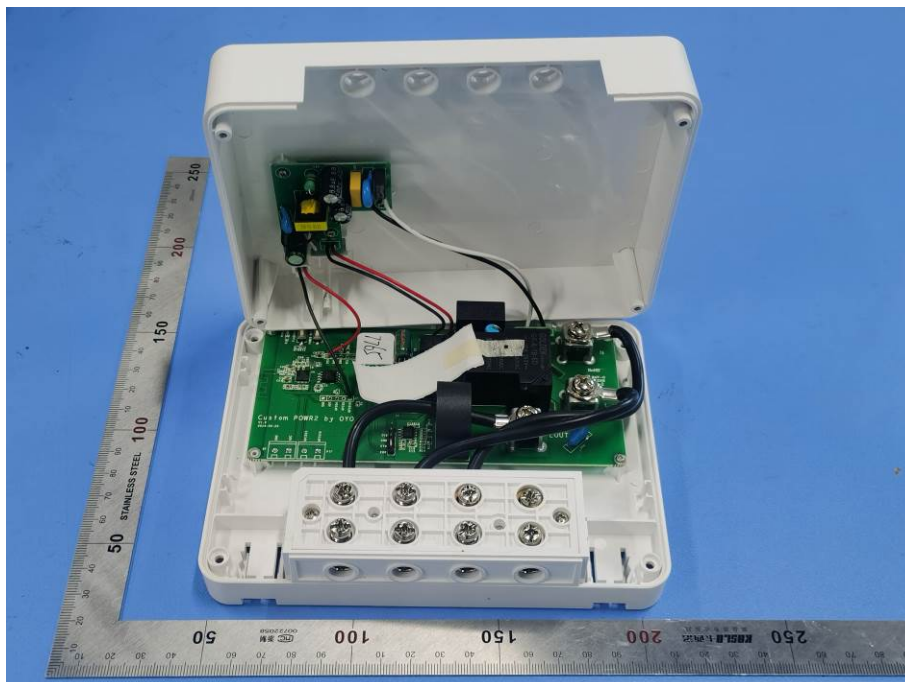


Figure 3 Internal View

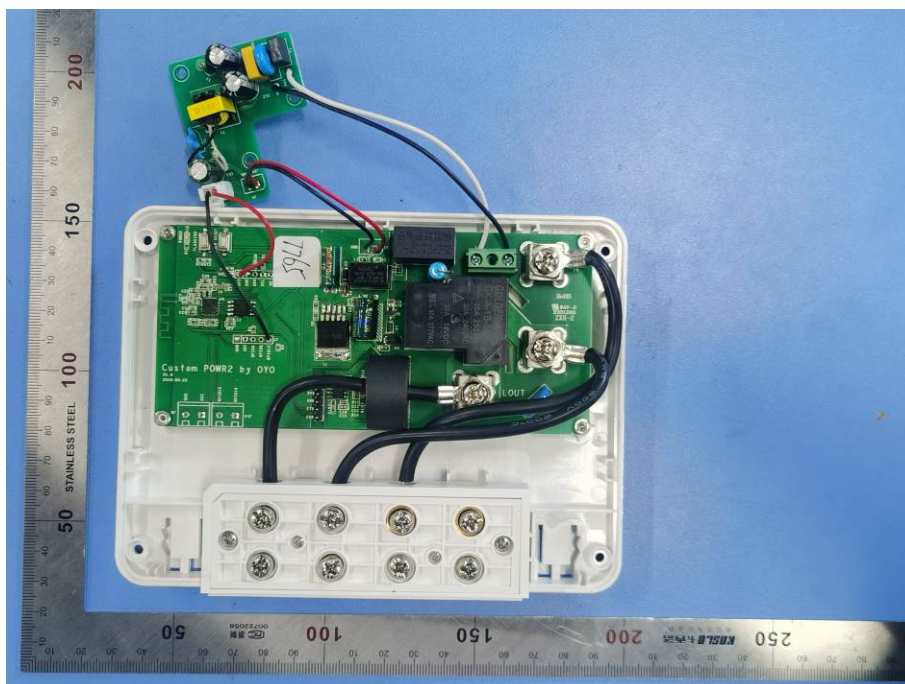


Figure 4 Internal View



ATTACHMENT 1

Photo Documentation

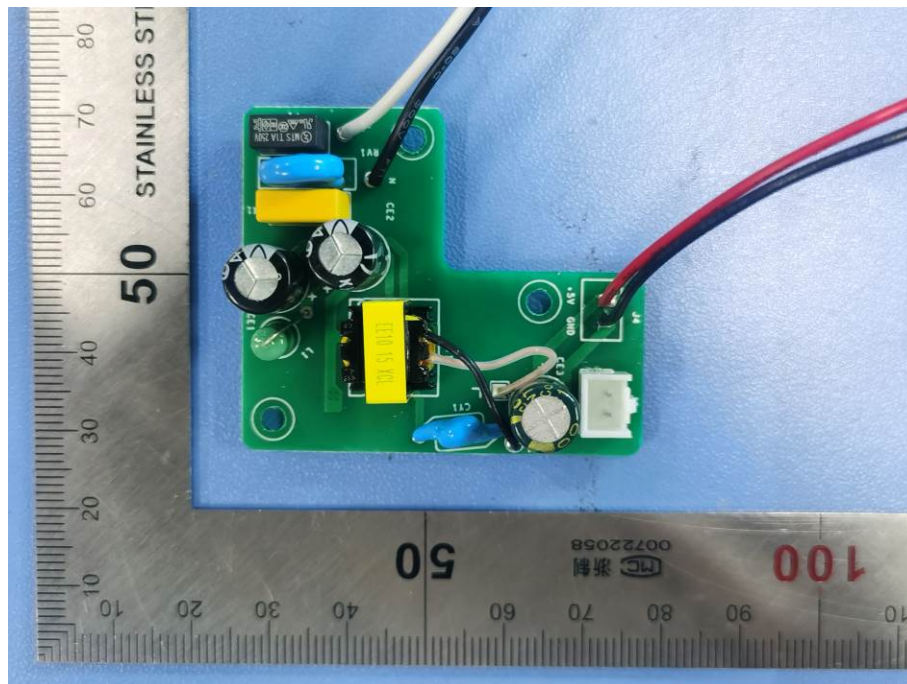


Figure 5 Internal View

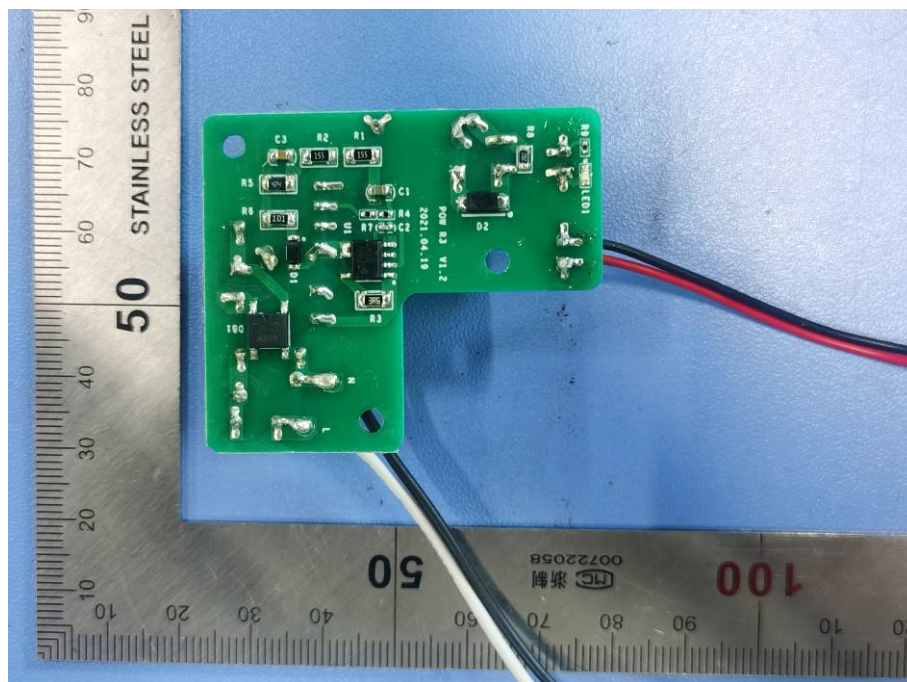


Figure 6 Internal View



ATTACHMENT 1

Photo Documentation

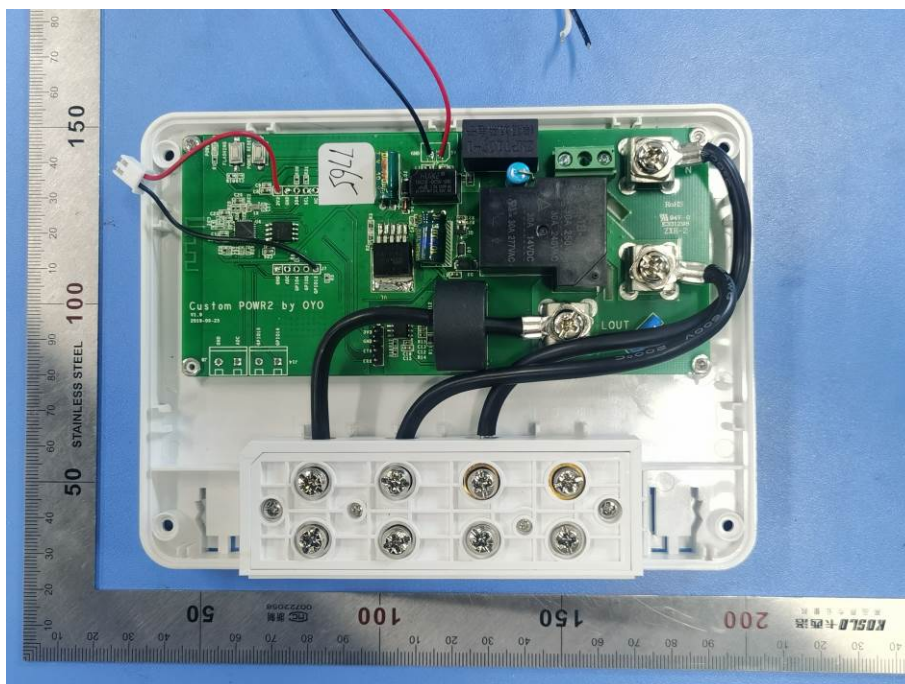


Figure 7 Internal View

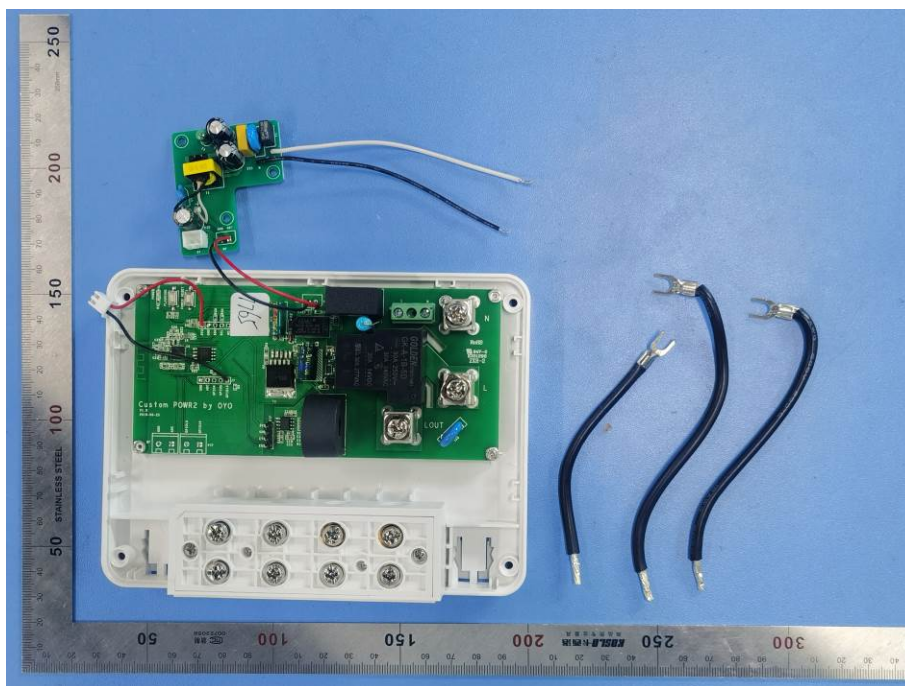


Figure 8 Internal View



ATTACHMENT 1

Photo Documentation

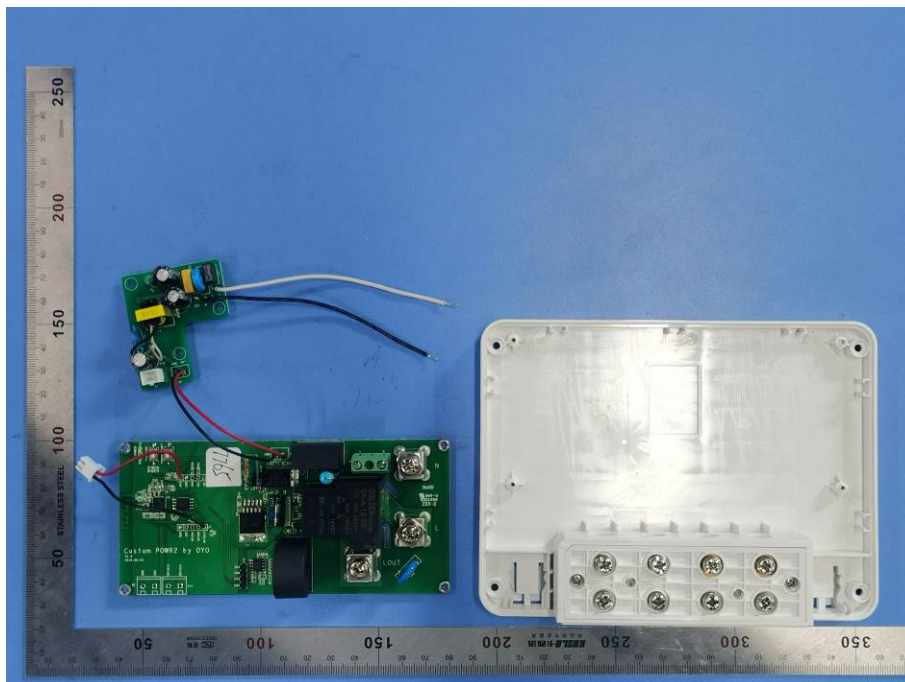


Figure 9 Internal View

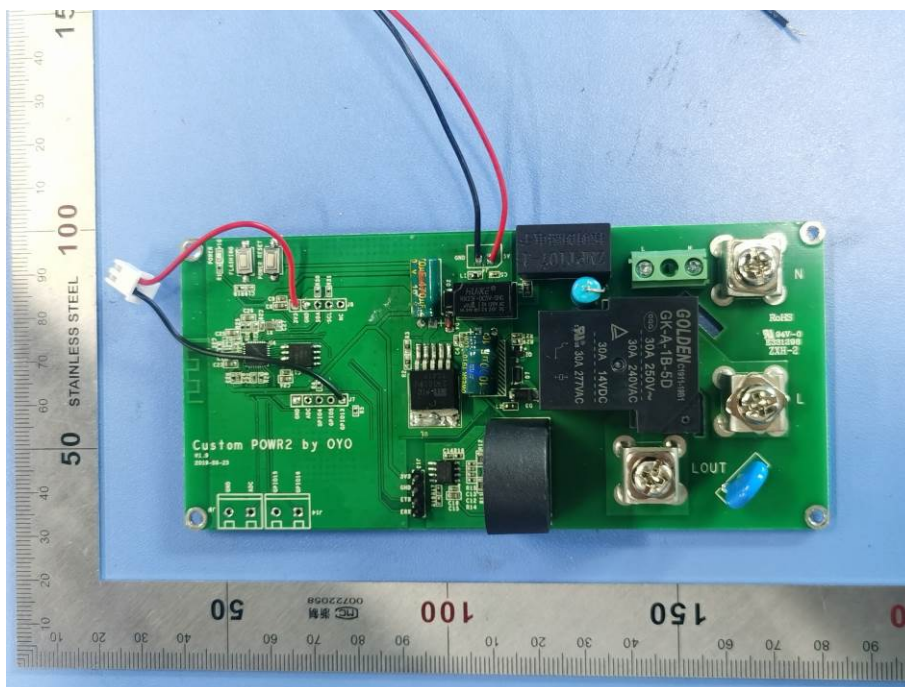


Figure 10 Internal View



ATTACHMENT 1

Photo Documentation

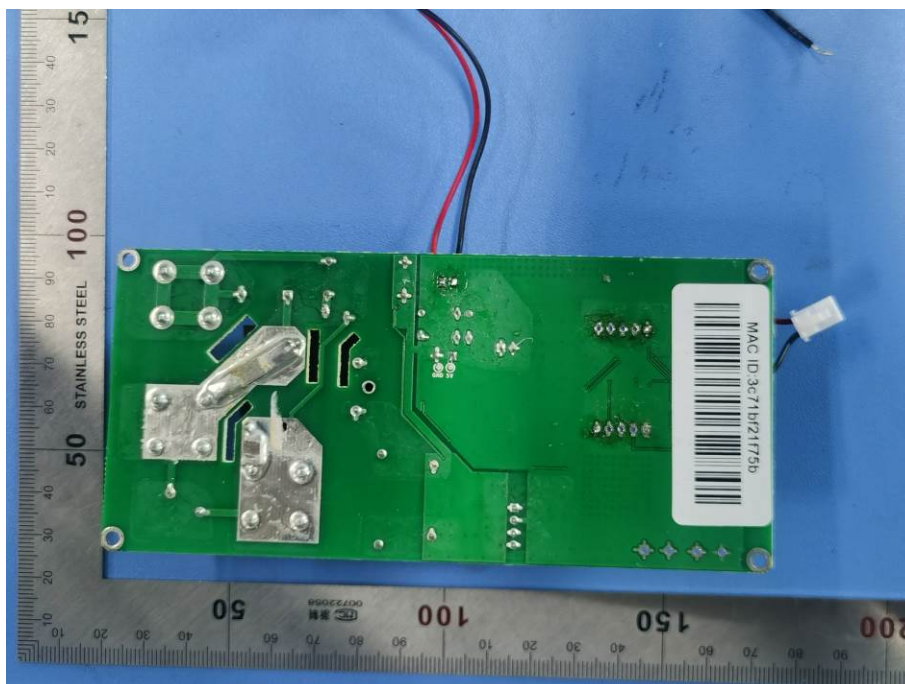


Figure 11 Internal View

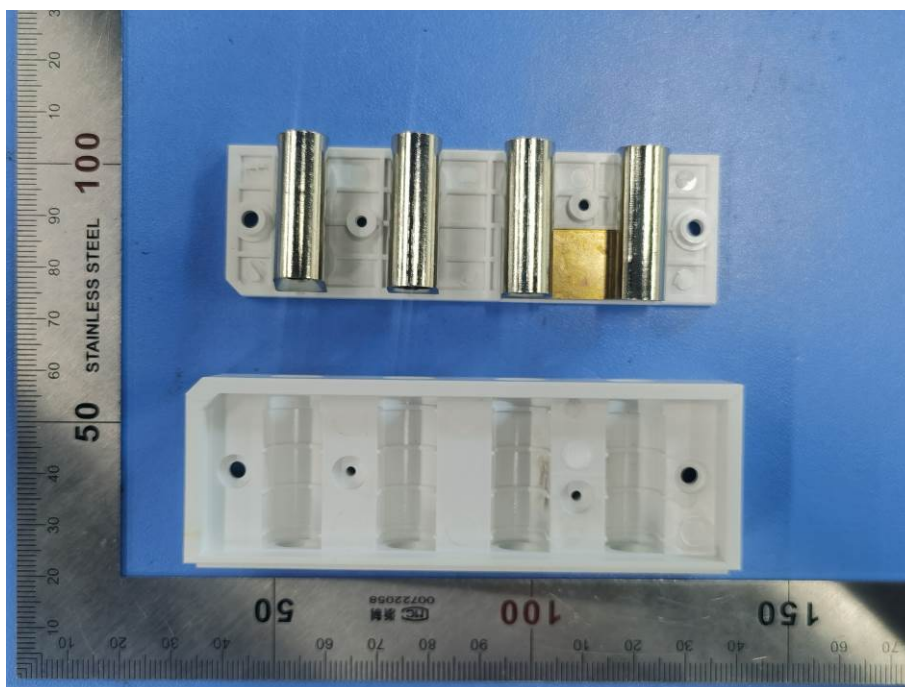


Figure 12 Internal View

--- END OF REPORT ---